

(19)



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11)

EP 1 360 967 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
12.11.2003 Bulletin 2003/46

(51) Int Cl.7: **A61L 31/10, A61L 31/16,
A61F 2/06**

(21) Application number: **03252701.2**

(22) Date of filing: **29.04.2003**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR**
Designated Extension States:
AL LT LV MK

(72) Inventors:
• **Davila, Luis A.**
Pleasanton, CA 94588 (US)
• **Wilson, David J.**
Branchburg, NJ 08876 (US)

(30) Priority: **30.04.2002 US 136569**

(74) Representative: **Belcher, Simon James**
Urquhart-Dykes & Lord
Tower House
Merrion Way
Leeds LS2 8PA (GB)

(71) Applicant: **Cordis Corporation**
Miami Lakes Florida 33014 (US)

(54) **Coated medical devices**

(57) A stent-graft for implantation into a treatment site of a living organism, comprises a scaffold structure for maintaining luminal patency and a graft material secured to at least a portion of the scaffold structure. A biocompatible vehicle is affixed to at least one of the scaffold structure and graft material, and at least one therapeutic agent is incorporated into the biocompatible vehicle for the treatment of a disease condition. The

therapeutic drugs, agents or compounds can further reduce a biological organism's reaction to the introduction of the stent-graft to the organism. Various materials and coating techniques can be utilised to maintain the drugs, agents or compounds on the stent-graft device while it is delivered and positioned.

BEST AVAILABLE COPY

EP 1 360 967 A1

ATTORNEY DOCKET NUMBER: 10177-191-999
SERIAL NUMBER: 10/603,115
REFERENCE: **B46**

(19)



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11)

EP 1 360 967 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:

12.11.2003 Bulletin 2003/46

(51) Int Cl.7: **A61L 31/10, A61L 31/16,
A61F 2/06**

(21) Application number: **03252701.2**

(22) Date of filing: **29.04.2003**

(84) Designated Contracting States:

**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR**

Designated Extension States:

AL LT LV MK

(72) Inventors:

- Davila, Luis A.
Pleasanton, CA 94588 (US)
- Wilson, David J.
Branchburg, NJ 08876 (US)

(30) Priority: **30.04.2002 US 136569**

(71) Applicant: **Cordis Corporation
Miami Lakes Florida 33014 (US)**

(74) Representative: **Belcher, Simon James
Urquhart-Dykes & Lord
Tower House
Merrion Way
Leeds LS2 8PA (GB)**

(54) **Coated medical devices**

(57) A stent-graft for implantation into a treatment site of a living organism, comprises a scaffold structure for maintaining luminal patency and a graft material secured to at least a portion of the scaffold structure. A biocompatible vehicle is affixed to at least one of the scaffold structure and graft material, and at least one therapeutic agent is incorporated into the biocompatible vehicle for the treatment of a disease condition. The

therapeutic drugs, agents or compounds can further reduce a biological organism's reaction to the introduction of the stent-graft to the organism. Various materials and coating techniques can be utilised to maintain the drugs, agents or compounds on the stent-graft device while it is delivered and positioned.

EP 1 360 967 A1

Description

[0001] The present invention relates to a stent-graft for implantation into a treatment site of a living organism, and to a system for bypassing an aneurysm.

[0002] The invention is concerned with the local administration of drug and drug combinations for the prevention and treatment of vascular disease, and more particularly to intraluminal medical devices for the local delivery of drug/drug combinations for the prevention and treatment of vascular disease caused by injury and methods for maintaining the drug/drug combinations on the intraluminal medical devices. The present invention also relates to medical devices having drugs, agents and/or compounds affixed thereto to treat and prevent disease and minimise or substantially eliminate a biological organism's reaction to the introduction of the medical device to the organism. In addition, the drugs, agents and/or compounds may be utilised to promote healing.

[0003] Many individuals suffer from circulatory disease caused by a progressive blockage of the blood vessels that profuse the heart and other major organs. More severe blockage of blood vessels in such individuals often leads to hypertension, ischemic injury, stroke, or myocardial infarction. Atherosclerotic lesions, which limit or obstruct coronary blood flow, are the major cause of ischemic heart disease. Percutaneous transluminal coronary angioplasty is a medical procedure whose purpose is to increase blood flow through an artery. Percutaneous transluminal coronary angioplasty is the predominant treatment for coronary vessel stenosis. The increasing use of this procedure is attributable to its relatively high success rate and its minimal invasiveness compared with coronary bypass surgery. A limitation associated with percutaneous transluminal coronary angioplasty is the abrupt closure of the vessel which may occur immediately after the procedure and restenosis which occurs gradually following the procedure. Additionally, restenosis is a chronic problem in patients who have undergone saphenous vein bypass grafting. The mechanism of acute occlusion appears to involve several factors and may result from vascular recoil with resultant closure of the artery and/or deposition of blood platelets and fibrin along the damaged length of the newly opened blood vessel.

[0004] Restenosis after percutaneous transluminal coronary angioplasty is a more gradual process initiated by vascular injury. Multiple processes, including thrombosis, inflammation, growth factor and cytokine release, cell proliferation, cell migration and extracellular matrix synthesis each contribute to the restenotic process.

[0005] While the exact mechanism of restenosis is not completely understood, the general aspects of the restenosis process have been identified. In the normal arterial wall, smooth muscle cells proliferate at a low rate, approximately less than 0.1% per day. Smooth muscle cells in the vessel walls exist in a contractile phenotype

characterised by eighty to ninety percent of the cell cytoplasmic volume occupied with the contractile apparatus. Endoplasmic reticulum, Golgi, and free ribosomes are few and are located in the perinuclear region. Extracellular matrix surrounds the smooth muscle cells and is rich in heparin-like glycosaminoglycans which are believed to be responsible for maintaining smooth muscle cells in the contractile phenotypic state (Campbell and Campbell, 1985).

[0006] Upon pressure expansion of an intracoronary balloon catheter during angioplasty, smooth muscle cells within the vessel wall become injured, initiating a thrombotic and inflammatory response. Cell derived growth factors such as platelet derived growth factor, basic fibroblast growth factor, epidermal growth factor, thrombin, etc., released from platelets, invading macrophages and/or leukocytes, or directly from the smooth muscle cells provoke a proliferative and migratory response in medial smooth muscle cells. These cells undergo a change from the contractile phenotype to a synthetic phenotype characterised by only a few contractile filament bundles, extensive rough endoplasmic reticulum, Golgi and free ribosomes. Proliferation/migration usually begins within one to two days post-injury and peaks several days thereafter (Campbell and Campbell, 1987; Clowes and Schwartz, 1985).

[0007] Daughter cells migrate to the intimal layer of arterial smooth muscle and continue to proliferate and secrete significant amounts of extracellular matrix proteins. Proliferation, migration and extracellular matrix synthesis continue until the damaged endothelial layer is repaired at which time proliferation slows within the intima, usually within seven to fourteen days post-injury. The newly formed tissue is called neointima. The further vascular narrowing that occurs over the next three to six months is due primarily to negative or constrictive remodelling.

[0008] Simultaneous with local proliferation and migration, inflammatory cells adhere to the site of vascular injury. Within three to seven days post-injury, inflammatory cells have migrated to the deeper layers of the vessel wall. In animal models employing either balloon injury or stent implantation, inflammatory cells may persist at the site of vascular injury for at least thirty days (Tanaka et al., 1993; Edelman et al., 1998). Inflammatory cells therefore are present and may contribute to both the acute and chronic phases of restenosis.

[0009] Numerous agents have been examined for presumed anti-proliferative actions in restenosis and have shown some activity in experimental animal models. Some of the agents which have been shown to successfully reduce the extent of intimal hyperplasia in animal models include: heparin and heparin fragments (Clowes, A.W. and Karnovsky M., *Nature* 265: 25-26, 1977; Guyton, J.R. et al., *Circ. Res.*, 46: 625-634, 1980; Clowes, A.W. and Clowes, M.M., *Lab. Invest.* 52: 611-616, 1985; Clowes, A.W. and Clowes, M.M., *Circ. Res.* 58: 839-845, 1986; Majesky et al., *Circ. Res.* 61:

296-300, 1987; Snow et al., Am. J. Pathol. 137: 313-330, 1990; Okada, T. et al., Neurosurgery 25: 92-98, 1989), colchicine (Currier, J.W. et al., Circ. 80: 11-66, 1989), taxol (Sollet, S.J. et al., J. Clin. Invest. 95: 1869-1876, 1995), angiotensin converting enzyme (ACE) inhibitors (Powell, J.S. et al., Science, 245: 186-188, 1989), angiopeptin (Lundergan, C.F. et al. Am. J. Cardiol. 17(Suppl. B):132B-136B, 1991), cyclosporin A (Jonasson, L. et al., Proc. Natl. Acad. Sci., 85: 2303, 1988), goat-anti-rabbit PDGF antibody (Ferns, G.A.A., et al., Science 253: 1129-1132, 1991), terbinafine (Nemecek, G.M. et al., J. Pharmacol. Exp. Thera. 248: 1167-1174, 1989), trapidil (Liu, M.W. et al., Circ. 81: 1089-1093, 1990), tranilast (Fukuyama, J. et al., Eur. J. Pharmacol. 318: 327-332, 1996), interferon-gamma (Hansson, G.K. and Holm, J., Circ. 84: 1266-1272, 1991), rapamycin (Marx, S.O. et al., Circ. Res. 76: 412-417, 1995), steroids (Colburn, M.D. et al., J. Vasc. Surg. 15: 510-518, 1992), see also Berk, B.C. et al., J. Am. Coll. Cardiol. 17: 111B-117B, 1991), ionizing radiation (Weinberger, J. et al., Int. J. Rad. Onc. Biol. Phys. 36: 767-775, 1996), fusion toxins (Farb, A. et al., Circ. Res. 80: 542-550, 1997) antisense oligonucleotides (Simons, M. et al., Nature 359: 67-70, 1992) and gene vectors (Chang, M.W. et al., J. Clin. Invest. 96: 2260-2268, 1995). Anti-proliferative action on smooth muscle cells *in vitro* has been demonstrated for many of these agents, including heparin and heparin conjugates, taxol, tranilast, colchicine, ACE inhibitors, fusion toxins, antisense oligonucleotides, rapamycin and ionizing radiation. Thus, agents with diverse mechanisms of smooth muscle cell inhibition may have therapeutic utility in reducing intimal hyperplasia.

[0010] However, in contrast to animal models, attempts in human angioplasty patients to prevent restenosis by systemic pharmacologic means have thus far been unsuccessful. Neither aspirin-dipyridamole, ticlopidine, anti-coagulant therapy (acute heparin, chronic warfarin, hirudin or hirulog), thromboxane receptor antagonism nor steroids have been effective in preventing restenosis, although platelet inhibitors have been effective in preventing acute reocclusion after angioplasty (Mak and Topol, 1997; Lang et al., 1991; Popma et al., 1991). The platelet GP IIb/IIIa receptor, antagonist, Reopro® is still under study but Reopro® has not shown definitive results for the reduction in restenosis following angioplasty and stenting. Other agents, which have also been unsuccessful in the prevention of restenosis, include the calcium channel antagonists, prostacyclin mimetics, angiotensin converting enzyme inhibitors, serotonin receptor antagonists, and anti-proliferative agents. These agents must be given systemically, however, and attainment of a therapeutically effective dose may not be possible; anti-proliferative (or anti-restenosis) concentrations may exceed the known toxic concentrations of these agents so that levels sufficient to produce smooth muscle inhibition may not be reached (Mak and Topol, 1997; Lang et al., 1991; Popma et al., 1991).

[0011] Additional clinical trials in which the effectiveness for preventing restenosis utilizing dietary fish oil supplements or cholesterol lowering agents has been examined showing either conflicting or negative results so that no pharmacological agents are as yet clinically available to prevent post-angioplasty restenosis (Mak and Topol, 1997; Franklin and Faxon, 1993; Serruys, P. W. et al., 1993). Recent observations suggest that the antilipid/antioxidant agent, probucol, may be useful in preventing restenosis but this work requires confirmation (Tardif et al., 1997; Yokoi, et al., 1997). Probucol is presently not approved for use in the United States and a thirty-day pretreatment period would preclude its use in emergency angioplasty. Additionally, the application of ionizing radiation has shown significant promise in reducing or preventing restenosis after angioplasty in patients with stents (Teirstein et al., 1997). Currently, however, the most effective treatments for restenosis are repeat angioplasty, atherectomy or coronary artery bypass grafting, because no therapeutic agents currently have Food and Drug Administration approval for use for the prevention of post-angioplasty restenosis.

[0012] Unlike systemic pharmacologic therapy, stents have proven useful in significantly reducing restenosis. Typically, stents are balloon-expandable slotted metal tubes (usually, but not limited to, stainless steel), which, when expanded within the lumen of an angio-plastied coronary artery, provide structural support through rigid scaffolding to the arterial wall. This support is helpful in maintaining vessel lumen patency. In two randomised clinical trials, stents increased angiographic success after percutaneous transluminal coronary angioplasty, by increasing minimal lumen diameter and reducing, but not eliminating, the incidence of restenosis at six months (Serruys et al., 1994; Fischman et al., 1994).

[0013] Additionally, the heparin coating of stents appears to have the added benefit of producing a reduction in sub-acute thrombosis after stent implantation (Serruys et al., 1996). Thus, sustained mechanical expansion of a stenosed coronary artery with a stent has been shown to provide some measure of restenosis prevention, and the coating of stents with heparin has demonstrated both the feasibility and the clinical usefulness of delivering drugs locally, at the site of injured tissue.

[0014] As stated above, the use of heparin coated stents demonstrates the feasibility and clinical usefulness of local drug delivery; however, the manner in which the particular drug or drug combination is affixed to the local delivery device will play a role in the efficacy of this type of treatment. For example, the processes and materials utilised to affix the drug/drug combinations to the local delivery device should not interfere with the operations of the drug/drug combinations. In addition, the processes and materials utilised should be biocompatible and maintain the drug/drug combinations on the local device through delivery and over a given period of time. For example, removal of the drug/drug combination during delivery of the local delivery device may

potentially cause failure of the device.

[0015] Accordingly, there exists a need for drug/drug combinations and associated local delivery devices for the prevention and treatment of vascular injury causing intimal thickening which is either biologically induced, for example, atherosclerosis, or mechanically induced, for example, through percutaneous transluminal coronary angioplasty. In addition, there exists a need for maintaining the drug/drug combinations on the local delivery device through delivery and positioning as well as ensuring that the drug/drug combination is released in therapeutic dosages over a given period of time.

[0016] A variety of stent coatings and compositions have been proposed for the prevention and treatment of injury causing intimal thickening. The coatings may be capable themselves of reducing the stimulus the stent provides to the injured lumen wall, thus reducing the tendency towards thrombosis or restenosis. Alternatively, the coating may deliver a pharmaceutical/therapeutic agent or drug to the lumen that reduces smooth muscle tissue proliferation or restenosis. The mechanism for delivery of the agent is through diffusion of the agent through either a bulk polymer or through pores that are created in the polymer structure, or by erosion of a biodegradable coating.

[0017] Both bioabsorbable and biostable compositions have been reported as coatings for stents. They generally have been polymeric coatings that either encapsulate a pharmaceutical/therapeutic agent or drug, e.g. rapamycin, taxol etc., or bind such an agent to the surface, e.g. heparin-coated stents. These coatings are applied to the stent in a number of ways, including, though not limited to, dip, spray, or spin coating processes.

[0018] One class of biostable materials that has been reported as coatings for stents is polyfluoro homopolymers. Polytetrafluoroethylene (PTFE) homopolymers have been used as implants for many years. These homopolymers are not soluble in any solvent at reasonable temperatures and therefore are difficult to coat onto small medical devices while maintaining important features of the devices (e.g. slots in stents).

[0019] Stents with coatings made from polyvinylidene fluoride homopolymers and containing pharmaceutical/therapeutic agents or drugs for release have been suggested. However, like most crystalline polyfluoro homopolymers, they are difficult to apply as high quality films onto surfaces without subjecting them to relatively high temperatures, that correspond to the melting temperature of the polymer.

[0020] It would be advantageous to develop coatings for implantable medical devices that will reduce thrombosis, restenosis, or other adverse reactions, that may include, but do not require, the use of pharmaceutical or therapeutic agents or drugs to achieve such affects, and that possess physical and mechanical properties effective for use in such devices even when such coated devices are subjected to relatively low maximum tem-

peratures. It would also be advantageous to develop implantable medical devices in combination with various drugs, agents and/or compounds which treat disease and minimise or substantially eliminate a living organisms' reaction to the implantation of the medical device.

[0021] The drug/drug combination therapies, drug/drug combination carriers and associated local delivery devices of the present invention provide a means for overcoming the difficulties associated with the methods and devices currently in use, as briefly described above. In addition, the methods for maintaining the drug/drug combination therapies, drug/drug combination carriers on the local delivery device ensure that the drug/drug combination therapies reach the target site.

[0022] In accordance with one aspect, the present invention is directed to a stent-graft for implantation into a treatment site of a living organism. The stent-graft comprises a scaffold structure for maintaining luminal patency, a graft material secured to at least a portion of the scaffold structure, a biocompatible vehicle affixed to at least one of the scaffold structures and graft material, and at least one agent in therapeutic dosages incorporated into the biocompatible vehicle for the treatment of a disease condition.

[0023] In accordance with another aspect, the present invention is directed to a stent-graft for implantation into a treatment site of a living organism. The stent-graft comprises first and second scaffold structures for maintaining luminal patency, a graft material sandwiched between the first and second scaffold structures, a biocompatible vehicle affixed to at least one of the first and second scaffold structures and the graft material, and at least one agent in therapeutic dosages incorporated into the biocompatible vehicle for the treatment of a disease condition.

[0024] In accordance with another aspect, the present invention is directed to a system for bypassing an aneurysm. The system comprises at least one prosthesis for establishing a fluid flow path through an aneurysmal section of artery, an anchoring element operatively associated with the at least one prosthesis for securing and sealing the at least one prosthesis upstream of the aneurysmal section of artery, a biocompatible vehicle affixed to at least one of the anchoring element and the at least one prosthesis, and at least one agent in therapeutic dosages incorporated into the biocompatible material for treatment of a disease condition.

[0025] The medical devices, drug coatings and methods for maintaining the drug coatings or vehicles thereon of the present invention utilises a combination of materials to treat disease, and reactions by living organisms due to the implantation of medical devices for the treatment of disease or other conditions. The local delivery of drugs, agents or compounds generally substantially reduces the potential toxicity of the drugs, agents or compounds when compared to systemic delivery while increasing their efficacy.

[0026] Drugs, agents or compounds may be affixed

to any number of medical devices to treat various diseases. The drugs, agents or compounds may also be affixed to minimise or substantially eliminate the biological organism's reaction to the introduction of the medical device utilised to treat a separate condition. For example, stents may be introduced to open coronary arteries or other body lumens such as biliary ducts. The introduction of these stents cause a smooth muscle cell proliferation-effect as well as inflammation. Accordingly, the stents may be coated with drugs, agents or compounds to combat these reactions. Anastomosis devices, routinely utilised in certain types of surgery, may also cause a smooth muscle cell proliferation effect as well as inflammation. Stent-grafts and systems utilizing stent-grafts, for example, aneurysm bypass systems may be coated with drugs, agents and/or compounds which prevent adverse affects caused by the introduction of these devices as well as to promote healing and incorporation. Therefore, the devices may also be coated with drugs, agents and/or compounds to combat these reactions.

[0027] The drugs, agents or compounds will vary depending upon the type of medical device, the reaction to the introduction of the medical device and/or the disease sought to be treated. The type of coating or vehicle utilised to immobilise the drugs, agents or compounds to the medical device may also vary depending on a number of factors, including the type of medical device, the type of drug, agent or compound and the rate of release thereof.

[0028] In order to be effective, the drugs, agents or compounds should preferably remain on the medical devices during delivery and implantation. Accordingly, various coating techniques for creating strong bonds between the drugs, agents or compounds may be utilised. In addition, various materials may be utilised as surface modifications to prevent the drugs, agents or compounds from coming off prematurely.

[0029] The drug/drug combinations and delivery devices of the present invention may be utilised to effectively prevent and treat vascular disease, and in particular, vascular disease caused by injury. Various medical treatment devices utilised in the treatment of vascular disease may ultimately induce further complications. For example, balloon angioplasty is a procedure utilised to increase blood flow through an artery and is the predominant treatment for coronary vessel stenosis. However, as stated above, the procedure typically causes a certain degree of damage to the vessel wall, thereby potentially exacerbating the problem at a point later in time. Although other procedures and diseases may cause similar injury, exemplary embodiments of the present invention will be described with respect to the treatment of restenosis and related complications following percutaneous transluminal coronary angioplasty and other similar arterial/venous procedures, including the joining of arteries, veins and other fluid carrying conduits.

[0030] While exemplary embodiments of the inven-

tion will be described with respect to the treatment of restenosis and related complications following percutaneous transluminal coronary angioplasty, it is important to note that the local delivery of drug/drug combinations may be utilised to treat a wide variety of conditions utilizing any number of medical devices, or to enhance the function and/or life of the device. For example, intraocular lenses, placed to restore vision after cataract surgery is often compromised by the formation of a secondary cataract. The latter is often a result of cellular overgrowth on the lens surface and can be potentially minimised by combining a drug or drugs with the device. Other medical devices which often fail due to tissue ingrowth or accumulation of proteinaceous material in, on and around the device, such as shunts for hydrocephalus, dialysis grafts, colostomy bag attachment devices, ear drainage tubes, leads for pace makers and implantable defibrillators can also benefit from the device-drug combination approach. Devices which serve to improve the structure and function of tissue or organ may also show benefits when combined with the appropriate agent or agents. For example, improved osteointegration of orthopaedic devices to enhance stabilisation of the implanted device could potentially be achieved by combining it with agents such as bone-morphogenic protein. Similarly other surgical devices, sutures, staples, anastomosis devices, vertebral disks, bone pins, suture anchors, hemostatic barriers, clamps, screws, plates, clips, vascular implants, tissue adhesives and sealants, tissue scaffolds, various types of dressings, bone substitutes, intraluminal devices, and vascular supports could also provide enhanced patient benefit using this drug-device combination approach. Essentially, any type of medical device may be coated in some fashion with a drug or drug combination which enhances treatment over use of the singular use of the device or pharmaceutical agent.

[0031] In addition to various medical devices, the coatings on these devices may be used to deliver therapeutic and pharmaceutic agents including: antiproliferative/antimitotic agents including natural products such as vinca alkaloids (i.e. vinblastine, vincristine, and vinorelbine), paclitaxel, epididophyllotoxins (i.e. etoposide, teniposide), antibiotics (daunorubicin (actinomycin D), daunorubicin, doxorubicin and idarubicin), anthracyclines, mitoxantrone, bleomycins, plicamycin (mitramycin) and mitomycin, enzymes (L-asparaginase which systemically metabolises L-asparagine and deprives cells which do not have the capacity to synthesise their own asparagine); antiplatelet agents such as G (GP) II_b/III_a inhibitors and vitronectin receptor antagonists; antiproliferative/antimitotic alkylating agents such as nitrogen mustards (mechlorethamine, cyclophosphamide and analogs, melphalan, chlorambucil), ethylenimines and methylmelamines (hexamethylmelamine and thiotepa), alkyl sulfonates-busulfan, nirtosoureas (carmustine (BCNU) and analogs, streptozocin), trazenes - dacarbazine (DTIC); antiproliferative/anti-

totic antimetabolites such as folic acid analogs (methotrexate), pyrimidine analogs (fluorouracil, floxuridine, and cytarabine), purine analogs and related inhibitors (mercaptopurine, thioguanine, pentostatin and 2-chlorodeoxyadenosine (cladribine)); platinum coordination complexes (cisplatin, carboplatin), procarbazine, hydroxyurea, mitotane, aminoglutethimide; hormones (i.e. estrogen); anticoagulants (heparin, synthetic heparin salts and other inhibitors of thrombin); fibrinolytic agents (such as tissue plasminogen activator, streptokinase and urokinase), aspirin, dipyridamole, ticlopidine, clopidogrel, abciximab; antimigratory; antisecretory (breveldin); anti-inflammatory: such as adrenocortical steroids (cortisol, cortisone, fludrocortisone, prednisone, prednisolone, 6 α -methylprednisolone, triamcinolone, betamethasone, and dexamethasone), non-steroidal agents (salicylic acid derivatives i.e. aspirin; para-aminophenol derivatives i.e. acetaminophen; indole and indene acetic acids (indomethacin, sulindac, and etodolac), heteroaryl acetic acids (tolmetin, diclofenac, and ketorolac), arylpropionic acids (ibuprofen and derivatives), anthranilic acids (mefenamic acid, and meclofenamic acid), enolic acids (piroxicam, tenoxicam, phenylbutazone, and oxyphenbutazone), nabumetone, gold compounds (auranofin, aurothioglucose, gold sodium thiomalate); immunosuppressives: (cyclosporine, tacrolimus (FK-506), sirolimus (rapamycin), azathioprine, mycophenolate mofetil); angiogenic agents: vascular endothelial growth factor (VEGF), fibroblast growth factor (FGF); angiotensin receptor blockers; nitric oxide donors; anti-sense oligonucleotides and combinations thereof; cell cycle inhibitors, mTOR inhibitors, and growth factor receptor signal transduction kinase inhibitors; retinoids; cyclin/CDK inhibitors; HMG co-enzyme reductase inhibitors (statins); and protease inhibitors.

[0032] As stated previously, the implantation of a coronary stent in conjunction with balloon angioplasty is highly effective in treating acute vessel closure and may reduce the risk of restenosis. Intravascular ultrasound studies (Mintz et al., 1996) suggest that coronary stenting effectively prevents vessel constriction and that most of the late luminal loss after stent implantation is due to plaque growth, probably related to neointimal hyperplasia. The late luminal loss after coronary stenting is almost two times higher than that observed after conventional balloon angioplasty. Thus, inasmuch as stents prevent at least a portion of the restenosis process, a combination of drugs, agents or compounds which prevents smooth muscle cell proliferation, reduces inflammation and reduces coagulation or prevents smooth muscle cell proliferation by multiple mechanisms, reduces inflammation and reduces coagulation combined with a stent may provide the most efficacious treatment for post-angioplasty restenosis. The systemic use of drugs, agents or compounds in combination with the local delivery of the same or different drug/drug combinations may also provide a beneficial treatment option.

[0033] The local delivery of drug/drug combinations

from a stent has the following advantages; namely, the prevention of vessel recoil and remodelling through the scaffolding action of the stent and the prevention of multiple components of neointimal hyperplasia or restenosis as well as a reduction in inflammation and thrombosis. This local administration of drugs, agents or compounds to stented coronary arteries may also have additional therapeutic benefit. For example, higher tissue concentrations of the drugs, agents or compounds may be achieved utilizing local delivery, rather than systemic administration. In addition, reduced systemic toxicity may be achieved utilizing local delivery rather than systemic administration while maintaining higher tissue concentrations. Also in utilizing local delivery from a stent rather than systemic administration, a single procedure may suffice with better patient compliance. An additional benefit of combination drug, agent, and/or compound therapy may be to reduce the dose of each of the therapeutic drugs, agents or compounds, thereby limiting their toxicity, while still achieving a reduction in restenosis, inflammation and thrombosis. Local stent-based therapy is therefore a means of improving the therapeutic ratio (efficacy/toxicity) of anti-restenosis, anti-inflammatory, anti-thrombotic drugs, agents or compounds.

[0034] There are a multiplicity of different stents that may be utilised following percutaneous transluminal coronary angioplasty. Although any number of stents may be utilised in accordance with the present invention, for simplicity, a limited number of stents will be described in exemplary embodiments of the present invention. The skilled artisan will recognise that any number of stents may be utilised in connection with the present invention. In addition, as stated above, other medical devices may be utilised.

[0035] A stent is commonly used as a tubular structure left inside the lumen of a duct to relieve an obstruction. Commonly, stents are inserted into the lumen in a non-expanded form and are then expanded autonomously, or with the aid of a second device *in situ*. A typical method of expansion occurs through the use of a catheter-mounted angioplasty balloon which is inflated within the stenosed vessel or body passageway in order to shear and disrupt the obstructions associated with the wall components of the vessel and to obtain an enlarged lumen.

[0036] Embodiments of the invention will now be described by way of example with reference to the accompanying drawings, in which:

Figure 1 is a view along the length of a stent (ends not shown) prior to expansion showing the exterior surface of the stent and the characteristic banding pattern.

Figure 2 is a perspective view along the length of the stent of Figure 1 having reservoirs in accordance with the present invention.

Figure 3 indicates the fraction of drug released as

a function of time from coatings of the present invention over which no topcoat has been disposed. Figure 4 indicates the fraction of drug released as a function of time from coatings of the present invention including a topcoat disposed thereon.

Figure 5 indicates the fraction of drug released as a function of time from coatings of the present invention over which no topcoat has been disposed. Figure 6 indicates *in vivo* stent release kinetics of rapamycin from poly(VDF/HFP).

Figure 7 is a cross-sectional view of a band of the stent of Figure 1 having drug coatings thereon in accordance with a first exemplary embodiment of the invention.

Figure 8 is a cross-sectional view of a band of the stent of Figure 1 having drug coatings thereon in accordance with a second exemplary embodiment of the invention.

Figure 9 is a cross-sectional view of a band of the stent of Figure 1 having drug coatings thereon in accordance with a third exemplary embodiment of the present invention.

Figures 10-13 illustrate an exemplary one-piece embodiment of an anastomosis device having a fastening flange and attached staple members in accordance with the present invention.

Figure 14 is a side view of an apparatus for joining anatomical structures together, according to an exemplary embodiment of the invention.

Figure 15 is a cross-sectional view showing a needle portion of the Figure 14 apparatus passing through edges of anatomical structures, according to an exemplary embodiment of the invention.

Figure 16 is a cross-sectional view showing the Figure 14 apparatus pulled through an anastomosis, according to an exemplary embodiment of the invention.

Figure 17 is a cross-sectional view showing a staple of the Figure 14 apparatus being placed into proximity with the anatomical structures, according to an exemplary embodiment of the invention.

Figure 18 is a cross-sectional view showing a staple of the Figure 14 apparatus being engaged on both sides of the anastomosis, according to an exemplary embodiment of the invention.

Figure 19 is a cross-sectional view showing a staple after it has been crimped to join the anatomical structures, according to an exemplary embodiment of the invention.

Figure 20 is a cross-sectional view of a balloon having a lubricious coating affixed thereto in accordance with the present invention.

Figure 21 is a cross-sectional view of a band of the stent in Figure 1 having a lubricious coating affixed thereto in accordance with the present invention.

Figure 22 is a partial cross-sectional view of a self-expanding stent in a delivery device having a lubricious coating in accordance with the present inven-

tion.

Figure 23 is a cross-sectional view of a band of the stent in Figure 1 having a modified polymer coating in accordance with the present invention.

Figure 24 is a side elevation of an exemplary stent-graft in accordance with the present invention.

Figure 25 is a fragmentary cross-sectional view of another alternate exemplary embodiment of a stent-graft in accordance with the present invention.

Figure 26 is a fragmentary cross-sectional view of another alternate exemplary embodiment of a stent-graft in accordance with the present invention.

Figure 27 is an elevation view of a fully deployed aortic repair system in accordance with the present invention.

Figure 28 is a perspective view of a stent for a first prosthesis, shown for clarity in an expanded state, in accordance with the present invention.

Figure 29 is a perspective view of a first prosthesis having a stent covered by a gasket material in accordance with the present invention.

[0037] Referring to the drawings, Figure 1 shows an exemplary stent 100 which comprises a fenestrated structure for placement in a blood vessel, duct or lumen to hold the vessel, duct or lumen open, more particularly for protecting a segment of artery from restenosis after angioplasty. The stent 100 may be expanded circumferentially and maintained in an expanded configuration, that is circumferentially or radially rigid. The stent 100 is axially flexible and when flexed at a band, the stent 100 avoids any externally protruding component parts.

[0038] The stent 100 generally comprises first and second ends with an intermediate section between them. The stent 100 has a longitudinal axis and comprises a plurality of longitudinally disposed bands 102, wherein each band 102 defines a generally continuous wave along a line segment parallel to the longitudinal axis. A plurality of circumferentially arranged links 104 maintain the bands 102 in a substantially tubular structure. Essentially, each longitudinally disposed band 102 is connected at a plurality of periodic locations, by a short circumferentially arranged link 104 to an adjacent band 102. The wave associated with each of the bands 102 has approximately the same fundamental spatial frequency in the intermediate section, and the bands 102 are so disposed that the wave associated with them are generally aligned so as to be generally in phase with one another. As illustrated in the figure, each longitudinally arranged band 102 undulates through approximately two cycles before there is a link to an adjacent band 102.

[0039] The stent 100 may be fabricated utilizing any number of methods. For example, the stent 100 may be fabricated from a hollow or formed stainless steel tube that may be machined using lasers, electric discharge milling, chemical etching or other means. The stent 100 is inserted into the body and placed at the desired site

in an unexpanded form. In one exemplary embodiment, expansion may be effected in a blood vessel by a balloon catheter, where the final diameter of the stent 100 is a function of the diameter of the balloon catheter used.

[0040] It should be appreciated that a stent 100 in accordance with the present invention may be embodied in a shape-memory material, including, for example, an appropriate alloy of nickel and titanium or stainless steel. Structures formed from stainless steel may be made self-expanding by configuring the stainless steel in a predetermined manner, for example, by twisting it into a braided configuration. In this embodiment after the stent 100 has been formed it may be compressed so as to occupy a space sufficiently small as to permit its insertion in a blood vessel or other tissue by insertion means, wherein the insertion means include a suitable catheter, or flexible rod. On emerging from the catheter, the stent 100 may be configured to expand into the desired configuration where the expansion is automatic or triggered by a change in pressure, temperature or electrical stimulation.

[0041] Figure 2 illustrates an exemplary embodiment of the present invention utilizing the stent 100 illustrated in Figure 1. As illustrated, the stent 100 may be modified to comprise one or more reservoirs 106. Each of the reservoirs 106 may be opened or closed as desired. These reservoirs 106 may be specifically designed to hold the drug/drug combinations to be delivered. Regardless of the design of the stent 100, it is preferable to have the drug/drug combination dosage applied with enough specificity and a sufficient concentration to provide an effective dosage in the lesion area. In this regard, the reservoir size in the bands 102 is preferably sized to adequately apply the drug/drug combination dosage at the desired location and in the desired amount.

[0042] In an alternate exemplary embodiment, the entire inner and outer surface of the stent 100 may be coated with drug/drug combinations in therapeutic dosage amounts. A detailed description of a drug for treating restenosis, as well as exemplary coating techniques, is described below. It is, however, important to note that the coating techniques may vary depending on the drug/drug combinations. Also, the coating techniques may vary depending on the material comprising the stent or other intraluminal medical device.

[0043] Rapamycin is a macrocyclic triene antibiotic produced by *Streptomyces hygroscopicus* as disclosed in US-3929992. It has been found that rapamycin among other things inhibits the proliferation of vascular smooth muscle cells *in vivo*. Accordingly, rapamycin may be utilised in treating intimal smooth muscle cell hyperplasia, restenosis, and vascular occlusion in a mammal, particularly following either biologically or mechanically mediated vascular injury, or under conditions that would predispose a mammal to suffering such a vascular injury. Rapamycin functions to inhibit smooth muscle cell proliferation and does not interfere with the re-endothelialisation of the vessel walls.

[0044] Rapamycin reduces vascular hyperplasia by antagonizing smooth muscle proliferation in response to mitogenic signals that are released during an angioplasty induced injury. Inhibition of growth factor and cytokine mediated smooth muscle proliferation at the late G1 phase of the cell cycle is believed to be the dominant mechanism of action of rapamycin. However, rapamycin is also known to prevent T-cell proliferation and differentiation when administered systemically. This is the basis for its immunosuppressive activity and its ability to prevent graft rejection.

[0045] As used herein, rapamycin includes rapamycin and all analogs, derivatives and congeners that bind to FKBP12, and other immunophilins and possesses the same pharmacologic properties as rapamycin including inhibition of TOR.

[0046] Although the anti-proliferative effects of rapamycin may be achieved through systemic use, superior results may be achieved through the local delivery of the compound. Essentially, rapamycin works in the tissues, which are in proximity to the compound, and has diminished effect as the distance from the delivery device increases. In order to take advantage of this effect, one would want the rapamycin in direct contact with the lumen walls. Accordingly, in a preferred embodiment, the rapamycin is incorporated onto the surface of the stent or portions thereof. Essentially, the rapamycin is preferably incorporated into the stent 100, illustrated in Figure 1, where the stent 100 makes contact with the lumen wall.

[0047] Rapamycin may be incorporated onto or affixed to the stent in a number of ways. In the exemplary embodiment, the rapamycin is directly incorporated into a polymeric matrix and sprayed onto the outer surface of the stent. The rapamycin elutes from the polymeric matrix over time and enters the surrounding tissue. The rapamycin preferably remains on the stent for at least three days up to approximately six months, and more preferably between seven and thirty days.

[0048] Any number of non-erodible polymers may be utilised in conjunction with the rapamycin. In one exemplary embodiment, the polymeric matrix comprises two layers. The base layer comprises a solution of poly(ethylene-co-vinylacetate) and polybutylmethacrylate. The rapamycin is incorporated into this base layer. The outer layer comprises only polybutylmethacrylate and acts as a diffusion barrier to prevent the rapamycin from eluting too quickly. The thickness of the outer layer or topcoat determines the rate at which the rapamycin elutes from the matrix. Essentially, the rapamycin elutes from the matrix by diffusion through the polymer matrix. Polymers are permeable, thereby allowing solids, liquids and gases to escape therefrom. The total thickness of the polymeric matrix is in the range from about one micron to about twenty microns or greater. It is important to note that primer layers and metal surface treatments may be utilised before the polymeric matrix is affixed to the medical device. For example, acid cleaning, alkaline (base)

cleaning, salinisation and parylene deposition may be used as part of the overall process described above.

[0049] The poly(ethylene-co-vinylacetate), polybutylmethacrylate and rapamycin solution may be incorporated into or onto the stent in a number of ways. For example, the solution may be sprayed onto the stent or the stent may be dipped into the solution. Other methods include spin coating and RF-plasma polymerisation. In one exemplary embodiment, the solution is sprayed onto the stent and then allowed to dry. In another exemplary embodiment, the solution may be electrically charged to one polarity and the stent electrically changed to the opposite polarity. In this manner, the solution and stent will be attracted to one another. In using this type of spraying process, waste may be reduced and more precise control over the thickness of the coat may be achieved.

[0050] In another exemplary embodiment, the rapamycin or other therapeutic agent may be incorporated into a film-forming polyfluoro copolymer comprising an amount of a first moiety selected from the group consisting of polymerised vinylidene fluoride and polymerised tetrafluoroethylene, and an amount of a second moiety other than the first moiety and which is copolymerised with the first moiety, thereby producing the polyfluoro copolymer, the second moiety being capable of providing toughness or elastomeric properties to the polyfluoro copolymer, wherein the relative amounts of the first moiety and the second moiety are effective to provide the coating and film produced therefrom with properties effective for use in treating implantable medical devices.

[0051] The present invention provides polymeric coatings comprising a polyfluoro copolymer and implantable medical devices, for example, stents coated with a film of the polymeric coating in amounts effective to reduce thrombosis and/or restenosis when such stents are used in, for example, angioplasty procedures. As used herein, polyfluoro copolymers means those copolymers comprising an amount of a first moiety selected from the group consisting of polymerised vinylidene fluoride and polymerised tetrafluoroethylene, and an amount of a second moiety other than the first moiety and which is copolymerised with the first moiety to produce the polyfluoro copolymer, the second moiety being capable of providing toughness or elastomeric properties to the polyfluoro copolymer, wherein the relative amounts of the first moiety and the second moiety are effective to provide coatings and film made from such polyfluoro copolymers with properties effective for use in coating implantable medical devices.

[0052] The coatings may comprise pharmaceutical or therapeutic agents for reducing restenosis, inflammation, and/or thrombosis, and stents coated with such coatings may provide sustained release of the agents. Films prepared from certain polyfluoro copolymer coatings of the present invention provide the physical and mechanical properties required of conventional coated

medical devices, even where maximum temperature, to which the device coatings and films are exposed, are limited to relatively low temperatures. This is particularly important when using the coating/film to deliver pharmaceutical/therapeutic agents or drugs that are heat sensitive, or when applying the coating onto temperature-sensitive devices such as catheters. When maximum exposure temperature is not an issue, for example, where heat-stable agents such as itraconazole are incorporated into the coatings, higher melting thermoplastic polyfluoro copolymers may be used and, if very high elongation and adhesion is required, elastomers may be used. If desired or required, the polyfluoro elastomers may be crosslinked by standard methods described in, e.g., *Modern Fluoropolymers*, (J. Shires ed.), John Wiley & Sons, New York, 1997, pp. 77-87.

[0053] The present invention comprises polyfluoro copolymers that provide improved biocompatible coatings or vehicles for medical devices. These coatings provide inert biocompatible surfaces to be in contact with body tissue of a mammal, for example, a human, sufficient to reduce restenosis, or thrombosis, or other undesirable reactions. While many reported coatings made from polyfluoro homopolymers are insoluble and/or require high heat, for example, greater than about 125°C to obtain films with adequate physical and mechanical properties for use on implantable devices, for example, stents, or are not particularly tough or elastomeric, films prepared from the polyfluoro copolymers of the present invention provide adequate adhesion, toughness or elasticity, and resistance to cracking when formed on medical devices. In certain exemplary embodiments, this is the case even where the devices are subjected to relatively low maximum temperatures.

[0054] The polyfluoro copolymers used for coatings according to the present invention are preferably film-forming polymers that have molecular weight high enough so as not to be waxy or tacky. The polymers and films formed therefrom should preferably adhere to the stent and not be readily deformable after deposition on the stent as to be able to be displaced by hemodynamic stresses. The polymer molecular weight should preferably be high enough to provide sufficient toughness so that films comprising the polymers will not be rubbed off during handling or deployment of the stent. In certain exemplary embodiments the coating will not crack where expansion of the stent or other medical devices occurs.

[0055] Coatings of the present invention comprise polyfluoro copolymers, as defined above. The second moiety polymerised with the first moiety to prepare the polyfluoro copolymer may be selected from those polymerised, biocompatible monomers that would provide biocompatible polymers acceptable for implantation in a mammal, while maintaining sufficient elastomeric film properties for use on medical devices claimed herein. Such monomers include, without limitation, hexafluoropropylene (HFP), tetrafluoroethylene (TFE), vinylidene-

fluoride, 1-hydropentafluoropropylene, perfluoro(methyl vinyl ether), chlorotrifluoroethylene (CTFE), pentafluoropropene, trifluoroethylene, hexafluoroacetone and hexafluoroisobutylene.

[0056] Polyfluoro copolymers used in the present invention typically comprise vinylidene fluoride copolymerised with hexafluoropropylene, in the weight ratio in the range of from about fifty to about ninety-two weight percent vinylidene fluoride to about fifty to about eight weight percent HFP. Preferably, polyfluoro copolymers used in the present invention comprise from about 50 to about 85 wt-% vinylidene fluoride copolymerised with from about 50 to about 15 wt-% HFP. More preferably, the polyfluoro copolymers will comprise from about 55 to about 70 wt-% vinylidene fluoride copolymerised with from about 55 to about 30 wt-% HFP. Even more preferably, polyfluoro copolymers comprise from about 55 to about 65 wt-% vinylidene fluoride copolymerised with from about 45 to about 35 wt-% HFP. Such polyfluoro copolymers are soluble, in varying degrees, in solvents such as dimethylacetamide (DMAc), tetrahydrofuran, dimethyl formamide, dimethyl sulphoxide and n-methyl pyrrolidone. Some are soluble in methylethylketone (MEK), acetone, methanol and other solvents commonly used in applying coatings to conventional implantable medical devices.

[0057] Conventional polyfluoro homopolymers are crystalline and difficult to apply as high quality films onto metal surfaces without exposing the coatings to relatively high temperatures that correspond to the melting temperature (T_m) of the polymer. The elevated temperature serves to provide films prepared from such PVDF homopolymer coatings that exhibit sufficient adhesion of the film to the device, while preferably maintaining sufficient flexibility to resist film cracking upon expansion/contraction of the coated medical device. Certain films and coatings according to the present invention provide these same physical and mechanical properties, or essentially the same properties, even when the maximum temperatures to which the coatings and films are exposed is less than about a maximum predetermined temperature. This is particularly important when the coatings/films comprise pharmaceutical or therapeutic agents or drugs that are heat sensitive, for example, subject to chemical or physical degradation or other heat-induced negative affects, or when coating heat sensitive substrates of medical devices, for example, subject to heat-induced compositional or structural degradation.

[0058] Depending on the particular device upon which the coatings and films of the present invention are to be applied and the particular use/result required of the device, polyfluoro copolymers used to prepare such devices may be crystalline, semi-crystalline or amorphous.

[0059] Where devices have no restrictions or limitations with respect to exposure of same to elevated temperatures, crystalline polyfluoro copolymers may be employed. Crystalline polyfluoro copolymers tend to resist

the tendency to flow under applied stress or gravity when exposed to temperatures above their glass transition (T_g) temperatures. Crystalline polyfluoro copolymers provide tougher coatings and films than their fully amorphous counterparts. In addition, crystalline polymers are more lubricious and more easily handled through crimping and transfer processes used to mount self-expanding stents, for example, formed from a nickel titanium based shape memory alloy (nitinol).

[0060] Semi-crystalline and amorphous polyfluoro copolymers are advantageous where exposure to elevated temperatures is an issue, for example, where heat-sensitive pharmaceutical or therapeutic agents are incorporated into the coatings and films, or where device design, structure and/or use preclude exposure to such elevated temperatures. Semi-crystalline polyfluoro copolymer elastomers comprising relatively high levels, for example, from about thirty to about forty-five weight percent of the second moiety, for example, HFP, copolymerised with the first moiety, for example, VDF, have the advantage of reduced coefficient of friction and self-blocking relative to amorphous polyfluoro copolymer elastomers. Such characteristics may be of significant value when processing, packaging and delivering medical devices coated with such polyfluoro copolymers. In addition, such polyfluoro copolymer elastomers comprising such relatively high content of the second moiety serves to control the solubility of certain agents, for example, rapamycin, in the polymer and therefore controls permeability of the agent through the matrix.

[0061] Polyfluoro copolymers utilised in the present inventions may be prepared by various known polymerisation methods. For example, high pressure, free-radical, semi-continuous emulsion polymerisation techniques such as those disclosed in Fluoroelastomers-dependence of relaxation phenomena on compositions, POLYMER 30, 2180, 1989, by Ajroldi, et al. may be employed to prepare amorphous polyfluoro copolymers, some of which may be elastomers. In addition, free-radical batch emulsion polymerisation techniques disclosed herein may be used to obtain polymers that are semi-crystalline, even where relatively high levels of the second moiety are included.

[0062] As described above, stents may comprise a wide variety of materials and a wide variety of geometries. Stents may be made of biocompatible materials, including biostable and bioabsorbable materials. Suitable biocompatible metals include, but are not limited to, stainless steel, tantalum, titanium alloys (including nitinol), and cobalt alloys (including cobalt-chromium nickel alloys). Suitable nonmetallic biocompatible materials include, but are not limited to, polyamides, polyolefins (i.e. polypropylene, polyethylene etc.), non-absorbable polyesters (i.e. polyethylene terephthalate), and bioabsorbable aliphatic polyesters (i.e. homopolymers and copolymers of lactic acid, glycolic acid, lactide, glycolide, para-dioxanone, trimethylene carbonate, ϵ -caprolactone, and blends thereof).

[0063] The film-forming biocompatible polymer coatings generally are applied to the stent in order to reduce local turbulence in blood flow through the stent, as well as adverse tissue reactions. The coatings and films formed therefrom also may be used to administer a pharmaceutically active material to the site of the stent placement. Generally, the amount of polymer coating to be applied to the stent will vary depending on, among other possible parameters, the particular polyfluoro copolymer used to prepare the coating, the stent design and the desired effect of the coating. Generally, the coated stent will comprise from about 0.1 to about fifteen weight percent of the coating, preferably from about 0.4 to about 10 wt-%. The polyfluoro copolymer coatings may be applied in one or more coating steps, depending on the amount of polyfluoro copolymer to be applied. Different polyfluoro copolymers may be used for different layers in the stent coating. In fact, in certain exemplary embodiments, it is highly advantageous to use a diluted first coating solution comprising a polyfluoro copolymer as a primer to promote adhesion of a subsequent polyfluoro copolymer coating layer that may include pharmaceutically active materials. The individual coatings may be prepared from different polyfluoro copolymers.

[0064] Additionally, a top coating may be applied to delay release of the pharmaceutical agent, or they could be used as the matrix for the delivery of a different pharmaceutically active material. Layering of coatings may be used to stage release of the drug or to control release of different agents placed in different layers.

[0065] Blends of polyfluoro copolymers may also be used to control the release rate of different agents or to provide a desirable balance of coating properties, i.e. elasticity, toughness, etc., and drug delivery characteristics, for example, release profile. Polyfluoro copolymers with different solubilities in solvents may be used to build up different polymer layers that may be used to deliver different drugs or to control the release profile of a drug. For example, polyfluoro copolymers comprising 85.5/14.5 (wt/wt) of poly(vinylidene fluoride)/HFP and 60.6/39.4 (wt/wt) of poly(vinylidene fluoride)/HFP are both soluble in DMAc. However, only the 60.6/39.4 PVDF polyfluoro copolymer is soluble in methanol. So, a first layer of the 85.5/14.5 PVDF polyfluoro copolymer comprising a drug could be over coated with a topcoat of the 60.6/39.4 PVDF polyfluoro copolymer made with the methanol solvent. The top coating may be used to delay the drug delivery of the drug contained in the first layer. Alternately, the second layer could comprise a different drug to provide for sequential drug delivery. Multiple layers of different drugs could be provided by alternating layers of first one polyfluoro copolymer, then the other. As will be readily appreciated by those skilled in the art, numerous layering approaches may be used to provide the desired drug delivery.

[0066] Coatings may be formulated by mixing one or more therapeutic agents with the coating polyfluoro co-

polymers in a coating mixture. The therapeutic agent may be present as a liquid, a finely divided solid, or any other appropriate physical form. Optionally, the coating mixture may include one or more additives, for example, nontoxic auxiliary substances such as diluents, carriers, excipients, stabilisers or the like. Other suitable additives may be formulated with the polymer and pharmaceutically active agent or compound. For example, a hydrophilic polymer may be added to a biocompatible hydrophobic coating to modify the release profile, or a hydrophobic polymer may be added to a hydrophilic coating to modify the release profile. One example would be adding a hydrophilic polymer selected from the group consisting of polyethylene oxide, polyvinyl pyrrolidone, polyethylene glycol, carboxymethyl cellulose, and hydroxymethyl cellulose to a polyfluoro copolymer coating to modify the release profile. Appropriate relative amounts may be determined by monitoring the *in vitro* and/or *in vivo* release profiles for the therapeutic agents.

[0067] The best conditions for the coating application are when the polyfluoro copolymer and pharmaceutical agent have a common solvent. This provides a wet coating that is a true solution. Less desirable, yet still usable, are coatings that contain the pharmaceutical agent as a solid dispersion in a solution of the polymer in solvent. Under the dispersion conditions, care must be taken to ensure that the particle size of the dispersed pharmaceutical powder, both the primary powder size and its aggregates and agglomerates, is small enough not to cause an irregular coating surface or to clog the slots of the stent that need to remain essentially free of coating. In cases where a dispersion is applied to the stent and the smoothness of the coating film surface requires improvement, or to be ensured that all particles of the drug are fully encapsulated in the polymer, or in cases where the release rate of the drug is to be slowed, a clear (polyfluoro copolymer only) topcoat of the same polyfluoro copolymer used to provide sustained release of the drug or another polyfluoro copolymer that further restricts the diffusion of the drug out of the coating may be applied. The topcoat may be applied by dip coating with mandrel to clear the slots. This method is disclosed in US-6153252. Other methods for applying the topcoat include spin coating and spray coating. Dip coating of the topcoat can be problematic if the drug is very soluble in the coating solvent, which swells the polyfluoro copolymer, and the clear coating solution acts as a zero concentration sink and redissolves previously deposited drug. The time spent in the dip bath may need to be limited so that the drug is not extracted out into the drug-free bath. Drying should be rapid so that the previously deposited drug does not completely diffuse into the topcoat.

[0068] The amount of therapeutic agent will be dependent upon the particular drug employed and medical condition being treated. Typically, the amount of drug represents about 0.001% to about 70% of the total coating weight, more typically about 0.001% to about 60%

of the total coating weight. It is possible that the drug may be present in amounts from 0.0001% of the total coating weight.

[0069] The quantity and type of polyfluoro copolymers employed in the coating film comprising the pharmaceutical agent will vary depending on the release profile desired and the amount of drug employed. The product may contain blends of the same or different polyfluoro copolymers having different molecular weights to provide the desired release profile or consistency to a given formulation.

[0070] Polyfluoro copolymers may release dispersed drug by diffusion. This can result in prolonged delivery (over, say approximately 1 to 2000 hours, preferably 2 to 800 hours) of effective amounts (0.001 mg/cm²-min to 1000 mg/cm²-min) of the drug. The dosage may be tailored to the subject being treated, the severity of the affliction, the judgment of the prescribing physician, and the like.

[0071] Individual formulations of drugs and polyfluoro copolymers may be tested in appropriate *in vitro* and *in vivo* models to achieve the desired drug release profiles. For example, a drug could be formulated with a polyfluoro copolymer, or blend of polyfluoro copolymers, coated onto a stent and placed in an agitated or circulating fluid system, for example, twenty-five percent ethanol in water. Samples of the circulating fluid could be taken to determine the release profile (such as by HPLC, UV analysis or use of radiotagged molecules). The release of a pharmaceutical compound from a stent coating into the interior wall of a lumen could be modelled in appropriate animal system. The drug release profile could then be monitored by appropriate means such as, by taking samples at specific times and assaying the samples for drug concentration (using HPLC to detect drug concentration). Thrombus formation can be modelled in animal models using the inplatelet imaging methods described by Hanson and Harker, Proc. Natl. Acad. Sci. USA 85:3184-3188 (1988). Following this or similar procedures, those skilled in the art will be able to formulate a variety of stent coating formulations.

[0072] While not a requirement of the present invention, the coatings and films may be crosslinked once applied to the medical devices. Crosslinking may be affected by any of the known crosslinking mechanisms, such as chemical, heat or light. In addition, cross-linking initiators and promoters may be used where applicable and appropriate. In those exemplary embodiments utilizing crosslinked films comprising pharmaceutical agents, curing may affect the rate at which the drug diffuses from the coating. Crosslinked polyfluoro copolymers films and coatings of the present invention also may be used without drug to modify the surface of implantable medical devices.

EXAMPLES

EXAMPLE 1:

[0073] A PVDF homopolymer (Solef® 1008 from Solvay Advanced Polymers, Houston, TX, T_m about 175°C) and polyfluoro copolymers of poly(vinylidene fluoride/HFP), 92/8 and 91/9 wt-% vinylidene fluoride/HFP as determined by F¹⁹ NMR, respectively (eg: Solef® 11010 and 11008, Solvay Advanced Polymers, Houston, TX, T_m about 159°C and 160°C, respectively) were examined as potential coatings for stents. These polymers are soluble in solvents such as, but not limited to, DMAc, N,N-dimethylformamide (DMF), dimethyl sulfoxide (DMSO), N-methylpyrrolidone (NMP), tetrahydrofuran (THF) and acetone. Polymer coatings were prepared by dissolving the polymers in acetone, at five weight percent as a primer, or by dissolving the polymer in 50/50 DMAc/acetone, at thirty weight percent as a topcoat. Coatings that were applied to the stents by dipping and dried at 60°C in air for several hours, followed by 60°C for three hours in a <100 mm Hg vacuum, resulted in white foamy films. As applied, these films adhered poorly to the stent and flaked off, indicating they were too brittle. When stents coated in this manner were heated above 175°C, i.e. above the melting temperature of the polymer, a clear, adherent film was formed. Since coatings require high temperatures, for example, above the melting temperature of the polymer, to achieve high quality films. As mentioned above, the high temperature heat treatment is unacceptable for the majority of drug compounds due to their thermal sensitivity.

EXAMPLE 2:

[0074] A polyfluoro copolymer (Solef® 21508) comprising 85.5wt-% vinylidene fluoride copolymerised with 14.5 wt-% HFP, as determined by F¹⁹ NMR, was evaluated. This copolymer is less crystalline than the polyfluoro homopolymer and copolymers described in Example 1. It also has a lower melting point reported to be about 133 °C. Once again, a coating comprising about 20 wt-% of the polyfluoro copolymer was applied from a polymer solution in 50/50 DMAc/MEK. After drying (in air) at 60°C for several hours, followed by 60°C for three hours in a <100 mtorr Hg vacuum, clear adherent films were obtained. This eliminated the need for a high temperature heat treatment to achieve high quality films. Coatings were smoother and more adherent than those of Example 1. Some coated stents that underwent expansion show some degree of adhesion loss and "tenting" as the film pulls away from the metal. Where necessary, modification of coatings containing such copolymers may be made, e.g. by addition of plasticisers or the like to the coating compositions. Films prepared from such coatings may be used to coat stents or other medical devices, particularly where those devices are not susceptible to expansion to the degree of the stents.

[0075] The coating process above was repeated, this time with a coating comprising the 85.5/14.6 (wt/wt) (vinylidene fluoride/HFP) and about 30 wt-% of rapamycin (Wyeth-Ayerst Laboratories, Philadelphia, PA), based on total weight of coating solids. Clear films that would occasionally crack or peel upon expansion of the coated stents resulted. It is believed that inclusion of plasticizers and the like in the coating composition will result in coatings and films for use on stents and other medical devices that are not susceptible to such cracking and peeling.

EXAMPLE 3:

[0076] Polyfluoro copolymers of still higher HFP content were then examined. This series of polymers were not semicrystalline, but rather are marketed as elastomers. One such copolymer is Fluorel™ FC2261Q (from Dyneon, a 3M-Hoechst Enterprise, Oakdale, MN), a 60.6/39.4 (wt/wt) copolymer of vinylidene fluoride/HFP. Although this copolymer has a T_g well below room temperature (T_g about -20°C) it is not tacky at room temperature or even at 60°C. This polymer has no detectable crystallinity when measured by differential scanning calorimetry (DSC) or by wide angle X-ray diffraction. Films formed on stents as described above were non-tacky, clear, and expanded without incident when the stents were expanded.

[0077] The coating process above was repeated, this time with coatings comprising the 60.6/39.4 (wt/wt) (vinylidene fluoride/HFP) and about 9, 30 and 50 wt-% of rapamycin (Wyeth-Ayerst Laboratories, Philadelphia, PA), based on total weight of coating solids, respectively. Coatings comprising about 9 and 30 wt-% rapamycin provided white, adherent, tough films that expanded without incident on the stent. Inclusion of 50% drug, in the same manner, resulted in some loss of adhesion upon expansion.

[0078] Changes in the comonomer composition of the polyfluoro copolymer also can affect the nature of the solid state coating, once dried. For example, the semicrystalline copolymer, Solef® 21508, containing 85.5 percent vinylidene fluoride polymerised with 14.5 wt-% HFP forms homogeneous solutions with about 30% rapamycin (drug weight divided by total solids weight, for example, drug plus copolymer) in DMAc and 50/50 DMAc/MEK. When the film is dried (60°C/16 hours followed by 60°C/3 hours in vacuum of 100 mm Hg) a clear coating, indicating a solid solution of the drug in the polymer, is obtained. Conversely, when an amorphous copolymer, Fluorel™ FC2261Q, of PDVF/HFP at 60.6/39.5 (wt/wt) forms a similar 30% solution of rapamycin in DMAc/MEK and is similarly dried, a white film, indicating phase separation of the drug and the polymer, is obtained. This second drug containing film is much slower to release the drug into an *in vitro* test solution of 25% ethanol in water than is the former clear film of crystalline Solef® 21508. X-ray analysis of both

films indicates that the drug is present in a non-crystalline form. Poor or very low solubility of the drug in the high HFP containing copolymer results in slow permeation of the drug through the thin coating film. Permeability is the product of diffusion rate of the diffusing species (in this case the drug) through the film (the copolymer) and the solubility of the drug in the film.

EXAMPLE 4: *In vitro* release results of rapamycin from coating.

[0079] Figure 3 is a plot of data for the 85.5/14.5 vinylidene fluoride/HFP polyfluoro copolymer, indicating fraction of drug released as a function of time, with no topcoat. Figure 4 is a plot of data for the same polyfluoro copolymer over which a topcoat has been disposed, indicating that most effect on release rate is with a clear topcoat. As shown therein, TC150 refers to a device comprising 150 µg of topcoat, TC235 refers to 235 µg of topcoat, etc. The stents before topcoating had an average of 750 µg of coating containing 30% rapamycin. Figure 5 is a plot for the 60.6/39.4 vinylidene fluoride/HFP polyfluoro copolymer, indicating fraction of drug released as a function of time, showing significant control of release rate from the coating without the use of a topcoat. Release is controlled by loading of drug in the film.

EXAMPLE 5: *In vivo* stent release kinetics of rapamycin from poly(VDF/HFP).

[0080] Nine New Zealand white rabbits (2.5-3.0 kg) on a normal diet were given aspirin 24 hours prior to surgery, again just prior to surgery and for the remainder of the study. At the time of surgery, animals were premedicated with Acepromazine (0.1-0.2 mg/kg) and anaesthetised with a Ketamine/Xylazine mixture (40 mg/kg and 5 mg/kg, respectively). Animals were given a single intraprocedural dose of heparin (150 IU/kg, i.v.)

[0081] Arterectomy of the right common carotid artery was performed and a 5 F catheter introducer (Cordis Inc) placed in the vessel and anchored with ligatures. Iodine contrast agent was injected to visualise the right common carotid artery, brachiocephalic trunk and aortic arch. A steerable guide wire (0.36 mm (0.014 inch)/180 cm, Cordis Inc) was inserted via the introducer and advanced sequentially into each iliac artery to a location where the artery possesses a diameter closest to 2 mm using the angiographic mapping done previously. Two stents coated with a film made of poly(VDF/HFP): (60.6/39.4) with 30% rapamycin were deployed in each animal where feasible, one in each iliac artery, using 3.0 mm balloon and inflation to 0.81 to 1.01 MPa (8 to 10 atmospheres) for thirty seconds followed after a one minute interval by a second inflation to 0.81 to 1.01 MPa (8 to 10 atmospheres) for 30 seconds. Follow-up angiographs visualizing both iliac arteries are obtained to confirm correct deployment position of the stent.

[0082] At the end of procedure, the carotid artery was

ligated and the skin is closed with 3/0 vicryl suture using a one layered interrupted closure. Animals were given butoropropanol (0.4 mg/kg, s.c.) and gentamycin (4 mg/kg; i.m.). Following recovery, the animals were returned to their cages and allowed free access to food and water.

[0083] Due to early deaths and surgical difficulties, two animals were not used in this analysis. Stented vessels were removed from the remaining seven animals at the following time points: one vessel (one animal) at ten minutes post implant; six vessels (three animals) between forty minutes and two hours post-implant (average, 1.2 hours); two vessels (two animals) at three days post implant; and two vessels (one animal) at seven days post-implant. In one animal at two hours, the stent was retrieved from the aorta rather than the iliac artery. Upon removal, arteries were carefully trimmed at both the proximal and distal ends of the stent. Vessels were then carefully dissected free of the stent, flushed to remove any residual blood, and both stent and vessel frozen immediately, wrapped separately in foil, labelled and kept frozen at -80°C. When all samples had been collected, vessels and stents were frozen, transported and subsequently analysed for rapamycin in tissue and results are illustrated in Figure 4.

EXAMPLE 6: Purifying the polymer.

[0084] The Fluorel™ FC2261Q copolymer was dissolved in MEK at about 10 wt-% and was washed in a 50/50 mixture of ethanol/water at a 14:1 of ethanol/water to MEK solution ratio. The polymer precipitated out and was separated from the solvent phase by centrifugation. The polymer again was dissolved in MEK and the washing procedure repeated. The polymer was dried after each washing step at 60°C in a vacuum oven (<200 mtorr) over night.

EXAMPLE 7: *In vivo* testing of coated stents in porcine coronary arteries.

[0085] CrossFlex™ stents (available from Cordis Inc) were coated with the "as received" Fluorel™ FC2261Q PVDF copolymer and with the purified polyfluoro copolymer of Example 6, using the dip and wipe approach. The coated stents were sterilised using ethylene oxide and a standard cycle. The coated stents and bare metal stents (controls) were implanted in porcine coronary arteries, where they remained for 28 days.

[0086] Angiography was performed on the pigs at implantation and at 28 days. Angiography indicated that the control uncoated stent exhibited about 21% restenosis. The polyfluoro copolymer "as received" exhibited about 26% restenosis (equivalent to the control) and the washed copolymer exhibited about 12.5% restenosis.

[0087] Histology results reported neointimal area at 28 days to be 2.89 ± 0.2 , 3.57 ± 0.4 and 2.75 ± 0.3 , respectively, for the bare metal control, the unpurified copolymer and the purified copolymer.

[0088] Since rapamycin acts by entering the surrounding tissue, it is preferably only affixed to the surface of the stent making contact with one tissue. Typically, only the outer surface of the stent makes contact with the tissue. Accordingly, in one exemplary embodiment, only the outer surface of the stent is coated with rapamycin.

[0089] The circulatory system, under normal conditions, has to be self-sealing, otherwise continued blood loss from an injury would be life threatening. Typically, all but the most catastrophic bleeding is rapidly stopped through a process known as hemostasis. Hemostasis occurs through a progression of steps. At high rates of flow, hemostasis is a combination of events involving platelet aggregation and fibrin formation. Platelet aggregation leads to a reduction in the blood flow due to the formation of a cellular plug while a cascade of biochemical steps leads to the formation of a fibrin clot.

[0090] Fibrin clots, as stated above, form in response to injury. There are certain circumstances where blood clotting or clotting in a specific area may pose a health risk. For example, during percutaneous transluminal coronary angioplasty, the endothelial cells of the arterial walls are typically injured, thereby exposing the sub-endothelial cells. Platelets adhere to these exposed cells. The aggregating platelets and the damaged tissue initiate further biochemical process resulting in blood coagulation. Platelet and fibrin blood clots may prevent the normal flow of blood to critical areas. Accordingly, there is a need to control blood clotting in various medical procedures. Compounds that do not allow blood to clot are called anti-coagulants. Essentially, an anti-coagulant is an inhibitor of thrombin formation or function. These compounds include drugs such as heparin and hirudin. As used herein, heparin includes all direct or indirect inhibitors of thrombin or Factor Xa.

[0091] In addition to being an effective anti-coagulant, heparin has also been demonstrated to inhibit smooth muscle cell growth *in vivo*. Thus, heparin may be effectively utilised in conjunction with rapamycin in the treatment of vascular disease. Essentially, the combination of rapamycin and heparin may inhibit smooth muscle cell growth via two different mechanisms in addition to the heparin acting as an anti-coagulant.

[0092] Because of its multifunctional chemistry, heparin may be immobilised or affixed to a stent in a number of ways. For example, heparin may be immobilised onto a variety of surfaces by various methods, including the photolink methods disclosed in US-3959078, US-4722906, US-5229172, US-5308641, US-5350800 and US-5415938. Heparinised surfaces have also been achieved by controlled release from a polymer matrix, for example, silicone rubber, as disclosed in US-5837313, US-6099562 and US-6120536.

[0093] Unlike rapamycin, heparin acts on circulating proteins in the blood and heparin need only make contact with blood to be effective. Accordingly, if used in conjunction with a medical device, such as a stent, it

would preferably be only on the side that comes into contact with the blood. For example, if heparin were to be administered via a stent, it would only have to be on the inner surface of the stent to be effective.

[0094] In an exemplary embodiment of the invention, a stent may be utilised in combination with rapamycin and heparin to treat vascular disease. In this exemplary embodiment, the heparin is immobilised to the inner surface of the stent so that it is in contact with the blood and the rapamycin is immobilised to the outer surface of the stent so that it is in contact with the surrounding tissue. Figure 7 illustrates a cross-section of a band 102 of the stent 100 illustrated in Figure 1. As illustrated, the band 102 is coated with heparin 108 on its inner surface 110 and with rapamycin 112 on its outer surface 114.

[0095] In an alternate exemplary embodiment, the stent may comprise a heparin layer immobilised on its inner surface, and rapamycin and heparin on its outer surface. Utilizing current coating techniques, heparin tends to form a stronger bond with the surface it is immobilised to than does rapamycin. Accordingly, it may be possible to first immobilise the rapamycin to the outer surface of the stent and then immobilise a layer of heparin to the rapamycin layer. In this embodiment, the rapamycin may be more securely affixed to the stent while still effectively eluting from its polymeric matrix, through the heparin and into the surrounding tissue. Figure 8 illustrates a cross-section of a band 102 of the stent 100 illustrated in Figure 1. As illustrated, the band 102 is coated with heparin 108 on its inner surface 110 and with rapamycin 112 and heparin 108 on its outer surface 114.

[0096] There are a number of possible ways to immobilise, i.e., entrapment or covalent linkage with an erodible bond, the heparin layer to the rapamycin layer. For example, heparin may be introduced into the top layer of the polymeric matrix. In other embodiments, different forms of heparin may be directly immobilised onto the top coat of the polymeric matrix, for example, as illustrated in Figure 9. As illustrated, a hydrophobic heparin layer 116 may be immobilised onto the top coat layer 118 of the rapamycin layer 112. A hydrophobic form of heparin is utilised because rapamycin and heparin coatings represent incompatible coating application technologies. Rapamycin is an organic solvent-based coating and heparin, in its native form, is a water-based coating.

[0097] As stated above, a rapamycin coating may be applied to stents by a dip, spray or spin coating method, and/or any combination of these methods. Various polymers may be utilised. For example, as described above, poly(ethylene-co-vinyl acetate) and polybutyl methacrylate blends may be utilised. Other polymers may also be utilised, but not limited to, for example, polyvinylidene fluoride-co-hexafluoropropylene and polyethylbutyl methacrylate-co-hexyl methacrylate. Also as described above, barrier or top coatings may also be applied to modulate the dissolution of rapamycin from the polymer matrix. In the exemplary embodiment de-

scribed above, a thin layer of heparin is applied to the surface of the polymeric matrix. Because these polymer systems are hydrophobic and incompatible with the hydrophilic heparin, appropriate surface modifications may be required.

[0098] The application of heparin to the surface of the polymeric matrix may be performed in various ways and utilizing various biocompatible materials. For example, in one embodiment, in water or alcoholic solutions, polyethylene imine may be applied on the stents, with care not to degrade the rapamycin (e.g., pH < 7, low temperature), followed by the application of sodium heparinate in aqueous or alcoholic solutions. As an extension of this surface modification, covalent heparin may be linked on polyethylene imine using amide-type chemistry (using a carbodiimide activator, e.g. EDC) or reductive amination chemistry (using CBAS-heparin and sodium cyanoborohydride for coupling). In another exemplary embodiment, heparin may be photolinked on the surface, if it is appropriately grafted with photo initiator moieties. Upon application of this modified heparin formulation on the covalent stent surface, light exposure causes cross-linking and immobilisation of the heparin on the coating surface. In yet another exemplary embodiment, heparin may be complexed with hydrophobic quaternary ammonium salts, rendering the molecule soluble in organic solvents (e.g. benzalkonium heparinate, troidodecylmethylammonium heparinate). Such a formulation of heparin may be compatible with the hydrophobic rapamycin coating, and may be applied directly on the coating surface, or in the rapamycin/ hydrophobic polymer formulation.

[0099] It is important to note that the stent, as described above, may be formed from any number of materials, including various metals, polymeric materials and ceramic materials. Accordingly, various technologies may be utilised to immobilise the various drugs, agent, compound combinations thereon. Specifically, in addition to the polymeric matrices described above biopolymers may be utilised. Biopolymers may be generally classified as natural polymers, while the above-described polymers may be described as synthetic polymers. Exemplary biopolymers, which may be utilised include, agarose, alginate, gelatin, collagen and elastin. In addition, the drugs, agents or compounds may be utilised in conjunction with other percutaneously delivered medical devices such as grafts and perfusion balloons.

[0100] In addition to utilizing an anti-proliferative and anti-coagulant, anti-inflammatories may also be utilised in combination therewith. One example of such a combination would be the addition of an anti-inflammatory corticosteroid such as dexamethasone with an anti-proliferative, such as rapamycin, cladribine, vincristine, taxol, or a nitric oxide donor and an anti-coagulant, such as heparin. Such combination therapies might result in a better therapeutic effect, i.e., less proliferation as well as less inflammation, a stimulus for proliferation, than would occur with either agent alone. The delivery of a

stent comprising an anti-proliferative, anti-coagulant, and an anti-inflammatory to an injured vessel would provide the added therapeutic benefit of limiting the degree of local smooth muscle cell proliferation, reducing a stimulus for proliferation, i.e., inflammation and reducing the effects of coagulation thus enhancing the restenosis-limiting action of the stent.

[0101] In other exemplary embodiments of the inventions, growth factor inhibitor or cytokine signal transduction inhibitor, such as the ras inhibitor, R115777, or P38 kinase inhibitor, RWJ67657, or a tyrosine kinase inhibitor, such as tyrphostin, might be combined with an anti-proliferative agent such as taxol, vincristine or rapamycin so that proliferation of smooth muscle cells could be inhibited by different mechanisms. Alternatively, an anti-proliferative agent such as taxol, vincristine or rapamycin could be combined with an inhibitor of extracellular matrix synthesis such as halofuginone. In the above cases, agents acting by different mechanisms could act synergistically to reduce smooth muscle cell proliferation and vascular hyperplasia. This invention is also intended to cover other combinations of two or more such drug agents. As mentioned above, such drugs, agents or compounds could be administered systemically, delivered locally via drug delivery catheter, or formulated for delivery from the surface of a stent, or given as a combination of systemic and local therapy.

[0102] In addition to anti-proliferatives, anti-inflammatories and anti-coagulants, other drugs, agents or compounds may be utilised in conjunction with the medical devices. For example, immunosuppressants may be utilised alone or in combination with these other drugs, agents or compounds. Also gene therapy, delivery mechanisms such as modified genes (nucleic acids including recombinant DNA) in viral vectors and non-viral gene vectors such as plasmids may also be introduced locally via a medical device. In addition, the present invention may be utilised with cell based therapy.

[0103] In addition to all of the drugs, agents, compounds and modified genes described above, chemical agents that are not ordinarily therapeutically or biologically active may also be utilised in conjunction with the present invention. These chemical agents, commonly referred to as pro-drugs, are agents that become biologically active upon their introduction into the living organism by one or more mechanisms. These mechanisms include the addition of compounds supplied by the organism or the cleavage of compounds from the agents caused by another agent supplied by the organism. Typically, pro-drugs are more absorbable by the organism. In addition, pro-drugs may also provide some additional measure of time release.

[0104] The coatings and drugs, agents or compounds described above may be utilised in combination with any number of medical devices, and in particular, with implantable medical devices such as stents and stent-grafts. Other devices such as vena cava filters and anastomosis devices may be used with coatings having

drugs, agents or compounds therein. The exemplary stent illustrated in Figures 1 and 2 is a balloon expandable stent. Balloon expandable stents may be utilised in any number of vessels or conduits, and are particularly well suited for use in coronary arteries. Self-expanding stents, on the other hand, are particularly well suited for use in vessels where crush recovery is a critical factor, for example, in the carotid artery. Accordingly, it is important to note that any of the drugs, agents or compounds, as well as the coatings described above, may be utilised in combination with self-expanding stents which are known in the art.

[0105] Anastomosis is the surgical joining of biological tissues, specifically the joining of tubular organs to create an intercommunication between them. Vascular surgery often involves creating an anastomosis between blood vessels or between a blood vessel and a vascular graft to create or restore a blood flow path to essential tissues. Coronary artery bypass graft surgery (CABG) is a surgical procedure to restore blood flow to ischemic heart muscle whose blood supply has been compromised by occlusion or stenosis of one or more of the coronary arteries. One method for performing CABG surgery involves harvesting a saphenous vein or other venous or arterial conduit from elsewhere in the body, or using an artificial conduit, such as one made of polyester (for example that sold under the trade mark Dacron) or polytetrafluoroethylene (such as that sold under the trade mark Goretex) tubing, and connecting this conduit as a bypass graft from a viable artery, such as the aorta, to the coronary artery downstream of the blockage or narrowing. A graft with both the proximal and distal ends of the graft detached is known as a "free graft". A second method involves rerouting a less essential artery, such as the internal mammary artery, from its native location so that it may be connected to the coronary artery downstream of the blockage. The proximal end of the graft vessel remains attached in its native position. This type of graft is known as a "pedicled graft". In the first case, the bypass graft must be attached to the native arteries by an end-to-side anastomosis at both the proximal and distal ends of the graft. In the second technique at least one end-to-side anastomosis must be made at the distal end of the artery used for the bypass. In the description of the exemplary embodiment given below reference will be made to the anastomoses on a free graft as the proximal anastomosis and the distal anastomosis. A proximal anastomosis is an anastomosis on the end of the graft vessel connected to a source of blood, for example, the aorta and a distal anastomosis is an anastomosis on the end of the graft vessel connected to the destination of the blood flowing through it, for example, a coronary artery. The anastomoses will also sometimes be called the first anastomosis or second anastomosis, which refers to the order in which the anastomoses are performed regardless of whether the anastomosis is on the proximal or distal end of the graft.

[0106] At present, essentially all vascular anastomoses are performed by conventional hand suturing. Suturing the anastomoses is a time-consuming and difficult task, requiring much skill and practice on the part of the surgeon. It is important that each anastomosis provide a smooth, open flow path for the blood and that the attachment be completely free of leaks. A completely leak-free seal is not always achieved on the very first try. Consequently, there is a frequent need for resuturing of the anastomosis to close any leaks that are detected.

[0107] The time consuming nature of hand sutured anastomoses is of special concern in CABG surgery for several reasons. Firstly, the patient is required to be supported on cardiopulmonary bypass (CPB) for most of the surgical procedure, the heart must be isolated from the systemic circulation (i.e. "cross-clamped"), and the heart must usually be stopped, typically by infusion of cold cardioplegia solution, so that the anastomosis site on the heart is still and blood-free during the suturing of the anastomosis. Cardiopulmonary bypass, circulatory isolation and cardiac arrest are inherently very traumatic, and it has been found that the frequency of certain post-surgical complications varies directly with the duration for which the heart is under cardioplegic arrest (frequently referred to as the "crossclamp time"). Secondly, because of the high cost of cardiac operating room time, any prolongation of the surgical procedure can significantly increase the cost of the bypass operation to the hospital and to the patient. Thus, it is desirable to reduce the duration of the crossclamp time and of the entire surgery by expediting the anastomosis procedure without reducing the quality or effectiveness of the anastomoses.

[0108] The already high degree of manual skill required for conventional manually sutured anastomoses is even more elevated for closed-chest or port-access thoracoscopic bypass surgery, a newly developed surgical procedure designed to reduce the morbidity of CABG surgery as compared to the standard open-chest CABG procedure. In the closed-chest procedure, surgical access to the heart is made through narrow access ports made in the intercostal spaces of the patient's chest, and the procedure is performed under thoracoscopic observation. Because the patient's chest is not opened, the suturing of the anastomoses must be performed at some distance, using elongated instruments positioned through the access ports for approximating the tissues and for holding and manipulating the needles and sutures used to make the anastomoses. This requires even greater manual skill than the already difficult procedure of suturing anastomoses during open-chest CABG surgery.

[0109] In order to reduce the difficulty of creating the vascular anastomoses during either open or closed-chest CABG surgery, it would be desirable to provide a rapid means for making a reliable end-to-side anastomosis between a bypass graft or artery and the aorta or the native vessels of the heart. A first approach to ex-

pediting and improving anastomosis procedures has been through stapling technology. Stapling technology has been successfully employed in many different areas of surgery for making tissue attachments faster and more reliably. The greatest progress in stapling technology has been in the area of gastrointestinal surgery. Various surgical stapling instruments have been developed for end-to-end, side-to-side, and end-to-side anastomoses of hollow or tubular organs, such as the bowel. These instruments, unfortunately, are not easily adaptable for use in creating vascular anastomoses. This is partially due to the difficulty in miniaturizing the instruments to make them suitable for smaller organs such as blood vessels. Possibly even more important is the necessity of providing a smooth, open flow path for the blood. Known gastrointestinal stapling instruments for end-to-side or end-to-end anastomosis of tubular organs are designed to create an inverted anastomosis, that is, one where the tissue folds inward into the lumen of the organ that is being attached. This is acceptable in gastrointestinal surgery, where it is most important to approximate the outer layers of the intestinal tract (the serosa). This is the tissue which grows together to form a strong, permanent connection. However, in vascular surgery this geometry is unacceptable for several reasons. Firstly, the inverted vessel walls would cause a disruption in the blood flow. This could cause decreased flow and ischemia downstream of the disruption, or, worse yet, the flow disruption or eddies created could become a locus for thrombosis which could shed emboli or occlude the vessel at the anastomosis site. Secondly, unlike the intestinal tract, the outer surfaces of the blood vessels (the adventitia) will not grow together when approximated. The sutures, staples, or other joining device may therefore be needed permanently to maintain the structural integrity of the vascular anastomosis. Thirdly, to establish a permanent, nonthrombogenic vessel, the innermost layer (the endothelium) should grow together for a continuous, uninterrupted lining of the entire vessel. Thus, it would be preferable to have a stapling instrument that would create vascular anastomoses that are everted, that is folded outward, or which create direct edge-to-edge coaptation without inversion.

[0110] At least one stapling instrument has been applied to performing vascular anastomoses during CABG surgery. This device, first adapted for use in CABG surgery by Vasilii Kolesov and later refined by Evgenii Kolesov (see US-4350160), was used to create an end-to-end anastomosis between the internal mammary artery (IMA) or a vein graft and one of the coronary arteries, primarily the left anterior descending coronary artery (LAD). Because the device could only perform end-to-end anastomoses, the coronary artery first had to be severed and dissected from the surrounding myocardium, and the exposed end everted for attachment. This technique limited the indications of the device to cases where the coronary artery was totally occluded, and therefore there was no loss of blood flow by completely

severing the coronary artery downstream of the blockage to make the anastomosis. Consequently, this device is not applicable where the coronary artery is only partially occluded and is not at all applicable to making the proximal side-to-end anastomosis between a bypass graft and the aorta.

[0111] One attempt to provide a vascular stapling device for end-to-side vascular anastomoses is disclosed in US-5234447. This document discloses a ring-shaped staple with staple legs extending from the proximal and distal ends of the ring to join two blood vessels together in an end-to-side anastomosis. However, the device does not provide a complete system for quickly and automatically performing an anastomosis. The method of applying the disclosed anastomosis staple involves a great deal of manual manipulation of the staple, using hand operated tools to individually deform the distal tines of the staple after the graft has been attached and before it is inserted into the opening made in the aortic wall. One of the more difficult manoeuvres in applying the staple involves carefully everting the graft vessel over the sharpened ends of the staple legs, then piercing the everted edge of the vessel with the staple legs. Experimental attempts to apply this technique have proven to be very problematic because of difficulty in manipulating the graft vessel and the potential for damage to the graft vessel wall. For speed, reliability and convenience, it is preferable to avoid the need for complex manoeuvres while performing the anastomosis. Further bending operations must then be performed on the staple legs. Once the distal tines of the staple have been deformed, it may be difficult to insert the staple through the aortotomy opening. Another disadvantage of the device is that the distal tines of the staple pierce the wall of the graft vessel at the point where it is everted over the staple. Piercing the wall of the graft vessel potentially invites leaking of the anastomosis and may compromise the structural integrity of the graft vessel wall, serving as a locus for a dissection or even a tear which could lead to catastrophic failure. Because the staple legs only apply pressure to the anastomosis at selected points, there is a potential for leaks between the staple legs. The distal tines of the staple are also exposed to the blood flow path at the anastomotic site where it is most critical to avoid the potential for thrombosis. There is also the potential that exposure of the medial layers of the graft vessel where the staple pierces the wall could be a site for the onset of intimal hyperplasia, which would compromise the long-term patency of the graft as described above. Because of these potential drawbacks, it is desirable to make the attachment to the graft vessel as atraumatic to the vessel wall as possible and to eliminate as much as possible the exposure of any foreign materials or any vessel layers other than a smooth uninterrupted intimal layer within the anastomosis site or within the graft vessel lumen.

[0112] A second approach to expediting and improving anastomosis procedures is through the use of anas-

tomotic fittings for joining blood vessels together. One attempt to provide a vascular anastomotic fitting device for end-to-side vascular anastomoses is disclosed in US-4366819. This device is a four-part anastomotic fitting having a tubular member over which the graft vessel is everted, a ring flange which engages the aortic wall from within the aortic lumen, and a fixation ring and a locking ring which engage the exterior of the aortic wall. Another similar anastomotic fitting is disclosed in US-4368736. This device is a tubular fitting with a flanged distal end that fastens to the aortic wall with an attachment ring, and a proximal end with a graft fixation collar for attaching to the graft vessel. These devices have a number of drawbacks. Firstly, the anastomotic fittings described expose the foreign material of the anastomotic device to the blood flow path within the arteries. This is undesirable because foreign materials within the blood flow path can have a tendency to cause hemolysis, platelet deposition and thrombosis. Immune responses to foreign material, such as rejection of the foreign material or auto-immune responses triggered by the presence of foreign material, tend to be stronger when the material is exposed to the bloodstream. As such, it is preferable that as much as possible of the interior surfaces of an anastomotic fitting that will be exposed to the blood flow path be covered with vascular tissue, either from the target vessel or from the graft vessel, so that a smooth, continuous, hemocompatible endothelial layer will be presented to the bloodstream. The anastomotic fitting disclosed in the '819 document also has the potential drawback that the spikes that hold the graft vessel onto the anastomotic fitting are very close to the blood flow path, potentially causing trauma to the blood vessel that could lead to leaks in the anastomosis or compromise of the mechanical integrity of the vessels. Consequently, it is desirable to provide an anastomosis fitting that is as atraumatic to the graft vessel as possible. Any sharp features such as attachment spikes should be placed as far away from the blood flow path and the anastomosis site as possible so that there is no compromise of the anastomosis seal or the structural integrity of the vessels.

[0113] Another device for end-to-end anastomosis designed for use in microsurgery, such as for reattaching vessels severed in accidents, is disclosed in US-4624257, US-4917090 and US-4917091, and sold by 3M under the trade mark UNILINK. This device provides an anastomosis clamp that has two eversion rings which are locked together by a series of impaling spikes on their opposing faces. However, this device is awkward for use in end-to-side anastomosis and tends to deform the target vessel; therefore it is not currently used in CABG surgery. Due to the delicate process needed to insert the vessels into the device, it would also be unsuitable for port-access surgery.

[0114] In order to solve these and other problems, it is desirable to provide an anastomosis device which performs an end-to-side anastomosis between blood

vessels or other hollow organs and vessels. It is also desirable to provide an anastomosis device which minimises the trauma to the blood vessels while performing the anastomosis, which minimises the amount of foreign materials exposed to the blood flow path within the blood vessels and which avoids leakage problems, and which promotes rapid endothelialisation and healing. It is also desirable that the invention provide a complete system for quickly and automatically performing an anastomosis with a minimal amount of manual manipulation.

[0115] Anastomosis devices may be utilised to join biological tissues, and more particularly, joining tubular organs to create a fluid channel. The connections between the tubular organs or vessels may be made side to side, end to end and/or end to side. Typically, there is a graft vessel and a target vessel. The target vessel may be an artery, vein or any other conduit or fluid carrying vessel, for example, coronary arteries. The graft vessel may comprise a synthetic material, an autologous vessel, a homologous vessel or a xenograft. Anastomosis devices may comprise any suitable biocompatible materials, for example, metals, polymers and elastomers. In addition, there are a wide variety of designs and configurations for anastomosis devices depending on the type of connection to be made. Similarly to stents, anastomosis devices cause some injury to the target vessel, thereby provoking a response from the body. Therefore, as in the case with stents, there is the potential for smooth muscle cell proliferation which can lead to blocked connections. Accordingly, there is a need to minimise or substantially eliminate smooth muscle cell proliferation and inflammation at the anastomotic site. Rapamycin and/or other drugs, agents or compounds may be utilised in a manner analogous to stents as described above. In other words, at least a portion of the anastomosis device may be coated with rapamycin or other drug, agent or compound.

[0116] Figures 10-13 illustrate an exemplary anastomosis device 200 for an end to side anastomosis. The exemplary anastomosis device 200 comprises a fastening flange 202 and attached staple members 204. As stated above, the anastomosis device may comprise any suitable biocompatible material. Preferably, the anastomosis device 200 comprises a deformable biocompatible metal, such as a stainless steel alloy, a titanium alloy or a cobalt alloy. Also as stated above, a surface coating or surface coating comprising a drug, agent or compound may be utilised to improve the biocompatibility or other material characteristics of the device as well as to reduce or substantially eliminate the body's response to its placement therein.

[0117] In the exemplary embodiment, the fastening flange 202 resides on the interior surface 206 of the target vessel wall 208 when the anastomosis is completed. In order to substantially reduce the risk of hemolysis, thrombogenesis or foreign body reactions, the total mass of the fastening flange 202 is preferably as small as possible to reduce the amount of foreign material

within the target vessel lumen 210.

[0118] The fastening flange 202 is in the form of a wire ring with an internal diameter, which when fully expanded, is slightly greater than the outside diameter of the graft vessel wall 214 and of the opening 216 made in the target vessel wall 208. Initially, the wire ring of the fastening flange 202 has a rippled wave-like shape to reduce the diameter of the ring so that it will easily fit through the opening 216 in the target vessel wall 208.

The plurality of staple members 204 extend substantially perpendicular from the wire ring in the proximal direction. In the illustrative exemplary embodiment, there are nine staple members 204 attached to the wire ring fastening flange 202. Other variations of the anastomosis device 200 might typically have from four to twelve staple members 204 depending on the size of the vessels to be joined and the security of attachment required in the particular application. The staple members 204 may be integrally formed with the wire ring fastening flange 202 or the staple members 204 may be attached to the fastening flange 202 by welding, brazing or any other suitable joining method. The proximal ends 218 of the staple members 204 are sharpened to easily pierce the target vessel wall 208 and the graft vessel wall 214. Preferably, the proximal ends 218 of the staple members 204 have barbs 220 to improve the security of the attachment when the anastomosis device 200 is deployed. The anastomosis device 200 is prepared for use by mounting the device onto the distal end of an application instrument 222. The fastening flange 202 is mounted on an anvil 224 attached to the distal end of the elongated shaft 226 of the application instrument 222. The staple members 204 are compressed inward against a conical holder 228 attached to the instrument 222 proximal to the anvil 224. The staple members 204 are secured in this position by a cap 230 which is slidably mounted on the elongated shaft 226. The cap 230 moves distally to cover the sharpened, barbed proximal ends 218 of the staple members 204 and to hold them against the conical holder 228. The application instrument 222 is then inserted through the lumen 232 of the graft vessel 214. This may be done by inserting the application instrument 222 through the graft vessel lumen 232 from the proximal to the distal end of the graft vessel 214, or it may be done by backloading the elongated shaft 226 of the application instrument 222 into the graft vessel lumen 232 from the distal end to the proximal end, whichever is most convenient in the case. The anvil 224 and conical holder 228 on the distal end of the application instrument 222 with the anastomosis device 200 attached is extended through the opening 216 into the lumen 210 of the target vessel.

[0119] Next, the distal end 234 of the graft vessel wall 214 is everted against the exterior surface 236 of the target vessel wall 208 with the graft vessel lumen 232 centred over the opening 216 in the target vessel wall 208. The cap 230 is withdrawn from the proximal ends 218 of the staple members 204, allowing the staple

members 204 to spring outward to their expanded position. The application instrument 222 is then drawn in the proximal direction so that the staple members pierce the target vessel wall 208 surrounding the opening 216 and the everted distal end 234 of the graft vessel 214.

[0120] The application instrument 222 has an annular staple former 238 which surrounds the outside of the graft vessel 214. Slight pressure on the everted graft vessel wall from the annular staple former 238 during the piercing step assists in piercing the staple members 204 through the graft vessel wall 214. Care should be taken not to apply too much pressure with the annular staple former 238 at this point in the process because the staple members 204 could be prematurely deformed before they have fully traversed the vessel walls. If desired, an annular surface made of a softer material, such as an elastomer, can be provided on the application instrument 222 to back up the vessel walls as the staple members 204 pierce through them.

[0121] Once the staple members 204 have fully traversed the target vessel wall 208 and the graft vessel wall 214, the staple former 238 is brought down with greater force while supporting the fastening flange 202 with the anvil 224. The staple members 204 are deformed outward so that the sharpened, barbed ends 218 pierce back through the everted distal end 234 and into the target vessel wall 208 to form a permanent attachment. To complete the anastomosis, the anvil 224 is withdrawn through the graft vessel lumen 232. As the anvil 224 passes through the wire ring fastening flange 202, it straightens out the wave-like ripples so that the wire ring flange 202 assumes its full expanded diameter. Alternately, the wire ring fastening flange 202 may be made of a resilient material so that the flange 202 may be compressed and held in a rippled or folded position until it is released within the target vessel lumen 210, whereupon it will resume its full expanded diameter. Another alternate construction would be to move the anastomosis device of a shape-memory alloy so that the fastening flange may be compressed and inserted through the opening in the target vessel, whereupon it would be returned to its full expanded diameter by heating the device 200 to a temperature above the shape-memory transition temperature.

[0122] In the above-described exemplary embodiment, the staple members 204 and/or the wire ring fastening flange 202 may be coated with any of the above-described agents, drugs or compounds such as rapamycin to prevent or substantially reduce smooth muscle wall proliferation.

[0123] Figure 14 illustrates an alternate exemplary embodiment of an anastomosis device. Figure 14 is a side view of an apparatus for joining at least two anatomical structures, according to another exemplary embodiment of the present invention. Apparatus 300 includes a suture 302 having a first end 304 and a second end 306, the suture 302 being constructed for passage through anatomical structures in a manner to be de-

scribed subsequently. Suture 302 may be formed from a wide variety of materials, for example, monofilament materials having minimal memory, including polypropylene or polyamide. Any appropriate diameter size may be used, for example, up to 8-0. Other suture types and sizes can be used.

[0124] A needle 308 preferably is curved and is disposed at the first end 304 of the suture 302. A sharp tip 310 of needle 308 enables easy penetration of various anatomical structures and enables the needle 308 and the suture 302 to pass through it readily. The needle 308 may be attached to the suture 302 in various ways, for example, by swedging, preferably substantially matching the outer diameter of the needle 308 and the suture 302 as closely as possible.

[0125] Apparatus 300 also includes a holding device 312 disposed at the second end 306 of the suture 302. The holding device 312 includes first and second limbs 314, 316, according to the illustrated exemplary embodiment, and preferably is of greater stiffness than the suture 302. The first limb 314 may be connected to suture 302 in a number of ways, for example, by swedging, preferably substantially matching the outside diameter of the suture 302 and the holding device 312 as closely as possible. The holding device 312 includes a staple structure comprising a bendable material that preferably is soft and malleable enough to crimp and hold its crimped position on the outside of an anastomosis. Such materials may include titanium or stainless steel. The holding device 312 may be referred to as a staple, according to the illustrated embodiment, and the suture 302 and the needle 308 a delivery system for staple 312.

[0126] Figure 14 illustrates one of the many possible initial configurations of holding device 312, i.e. the configuration the holding device 312 is in upon initial passage through the anatomical structures and/or at a point in time beforehand. As will be described, the holding device 312 is movable from the initial configuration to a holding configuration, in which holding device 312 holds the anatomical structures together. According to the illustrated exemplary embodiments, the holding device 312 assumes the holding configuration when it is bent or crimped, as shown in Figure 19 (further described below).

[0127] The holding device 312 preferably is substantially V-shaped or substantially U-shaped, as illustrated, but may assume a wide variety of shapes to suit particular surgical situations and/or surgeon preference. For example, one of limbs 314, 316 may be straight and the other curved, or limbs 314, 316 may be collinear. The holding device 312 preferably is as smooth and round in cross-section as the needle 308. Further, the diameters of the needle 308, the suture 302, and the holding device 312 preferably are substantially identical, especially the needle 308 and the holding device 312, to avoid creating holes in the anatomical structures that are larger than the diameter of the staple 312. Such holes likely would cause bleeding and/or leakage.

[0128] A method of using apparatus 300 is illustrated in Figures 15-19. First, as illustrated in Figure 15, the needle 308 passes through anatomical structures 318, 320, which are, for example, vascular structures. Specifically, according to the illustrated exemplary embodiment, the needle 308 passes through the edges 322, 324 of vascular structures 318, 320. Then, as shown in Figure 16, the needle 308 pulls suture 302 into and through both structures 318, 320. The staple 312 then is pulled into desired proximity with structures 318, 320, as shown in Figures 17-19, such that it is engaged on both sides of the illustrated anastomosis and associated lumen 326. According to one exemplary embodiment, traction is placed on suture 302 to hook staple 312 into position.

[0129] As illustrated in Figure 19 and as referenced earlier, the staple 312 then is moved from its initial configuration to a holding or crimped configuration 328, in which anatomical structures 318, 320 are joined together to effect an anastomosis between them. The staple 312 creates a substantially three hundred sixty-degree loop at the edge of the anastomosis, with crimped portion 330 outside lumen 321. A wide variety of tools and/or mechanisms may be used to crimp the staple 312 into its holding configuration, for example, in the manner of closure of a vascular clip. The same tool, or an alternative tool, may then be used to separate the staple 312 from the suture 302, for example, by cutting.

[0130] Thus, the staple 312 holds vascular structures 318, 320 together from inside the vascular structures, as well as from outside, unlike the many prior art staples that secure opposed structures only externally. This achieves a number of advantages, as described above. Not only does a better approximation result, but crimping a staple is simpler than tying one or more knots and is also less likely traumatic on tissue. Staple closure with a single crimp provides less tension on an anastomosis, for example, than a knot requiring several throws. Embodiments of the invention are especially advantageous in minimally invasive surgical situations, as knot-tying with, for example, a knot pusher in a minimally invasive setting through a small port is particularly tedious and can require up to four or five throws to prevent slippage. Crimping a staple through the port, as with embodiments of the invention, is far simpler and eliminates much of the difficulty.

[0131] According to one exemplary embodiment, the surgeon achieves a precise approximation of the vascular or other structures with preferably a limited number of staples or other holding devices, and then completes the anastomosis with biologic glue or laser techniques. The holding devices, for example, two or more in number, may be used to orient or line up the structures initially and thus used as a "pilot" for guiding the completion of the anastomosis.

[0132] In the above described exemplary embodiment, the holding device 312 may be coated with any of the above-described drugs, agents or compounds such

as rapamycin to prevent or substantially reduce smooth muscle cell proliferation.

[0133] As described above, various drugs, agents or compounds may be locally delivered via medical devices. For example, rapamycin and heparin may be delivered by a stent to reduce restenosis, inflammation, and coagulation. Various techniques for immobilizing the drugs, agents or compounds are discussed above, however, maintaining the drugs, agents or compounds on the medical devices during delivery and positioning is critical to the success of the procedure or treatment. For example, removal of the drug, agent or compound coating during delivery of the stent can potentially cause failure of the device. For a self-expanding stent, the retraction of the restraining sheath may cause the drugs, agents or compounds to rub off the stent. For a balloon expandable stent, the expansion of the balloon may cause the drugs, agents or compounds to simply delaminate from the stent through contact with the balloon or via expansion. Therefore, prevention of this potential problem is important to have a successful therapeutic medical device, such as a stent.

[0134] There are a number of approaches that may be utilised to substantially reduce the above-described concern. In one exemplary embodiment, a lubricant or mould release agent may be utilised. The lubricant or mould release agent may comprise any suitable biocompatible lubricious coating. An exemplary lubricious coating may comprise silicone. In this exemplary embodiment, a solution of the silicone base coating may be introduced onto the balloon surface, onto the polymeric matrix, and/or onto the inner surface of the sheath of a self-expanding stent delivery apparatus and allowed to air cure. Alternately, the silicone based coating may be incorporated into the polymeric matrix. It is important to note, however, that any number of lubricious materials may be utilised, with the basic requirements being that the material be biocompatible, that the material not interfere with the actions/effectiveness of the drugs, agents or compounds and that the material not interfere with the materials utilised to immobilise the drugs, agents or compounds on the medical device. It is also important to note that one or more, or all of the above-described approaches may be utilised in combination.

[0135] Referring now to Figure 20, there is illustrated a balloon 400 of a balloon catheter that may be utilised to expand a stent *in situ*. As illustrated, the balloon 400 comprises a lubricious coating 402. The lubricious coating 402 functions to minimise or substantially eliminate the adhesion between the balloon 400 and the coating on the medical device. In the exemplary embodiment described above, the lubricious coating 402 would minimise or substantially eliminate the adhesion between the balloon 400 and the heparin or rapamycin coating. The lubricious coating 402 may be attached to and maintained on the balloon 400 in any number of ways including but not limited to dipping, spraying, brushing

or spin coating of the coating material from a solution or suspension followed by curing or solvent removal step as needed.

[0136] Materials such as synthetic waxes, e.g. diethyleneglycol monostearate, hydrogenated castor oil, oleic acid, stearic acid, zinc stearate, calcium stearate, ethylenebis (stearamide), natural products such as paraffin wax, spermaceti wax, caruba wax, sodium alginate, ascorbic acid and flour, fluorinated compounds such as perfluoroalkanes, perfluorofatty acids and alcohol, synthetic polymers such as silicones e.g. polydimethylsiloxane, polytetrafluoroethylene, polyfluoroethers, polyalkylglycol e.g. polyethylene glycol waxes, and inorganic materials such as talc, kaolin, mica, and silica may be used to prepare these coatings. Vapour deposition polymerisation e.g. parylene-C deposition, or RF-plasma polymerisation of perfluoroalkenes and perfluoroalkanes can also be used to prepare these lubricious coatings.

[0137] Figure 21 illustrates a cross-section of a band 102 of the stent 100 illustrated in Figure 1. In this exemplary embodiment, the lubricious coating 500 is immobilised onto the outer surface of the polymeric coating. As described above, the drugs, agents or compounds may be incorporated into a polymeric matrix. The stent band 102 illustrated in Figure 21 comprises a base coat 502 comprising a polymer and rapamycin and a top coat 504 or diffusion layer 504 also comprising a polymer. The lubricious coating 500 is affixed to the top coat 502 by any suitable means, including but not limited to spraying, brushing, dipping or spin coating of the coating material from a solution or suspension with or without the polymers used to create the top coat, followed by curing or solvent removal step as needed. Vapour deposition polymerisation and RF-plasma polymerisation may also be used to affix those lubricious coating materials that lend themselves to this deposition method, to the top coating. In an alternate exemplary embodiment, the lubricious coating may be directly incorporated into the polymeric matrix.

[0138] If a self-expanding stent is utilised, the lubricious coating may be affixed to the inner surface of the restraining sheath. Figure 22 illustrates a partial cross-sectional view of self-expanding stent 200 within the lumen of a delivery apparatus sheath 14. As illustrated, a lubricious coating 600 is affixed to the inner surfaces of the sheath 14. Accordingly, upon deployment of the stent 200, the lubricious coating 600 preferably minimises or substantially eliminates the adhesion between the sheath 14 and the drug, agent or compound coated stent 200.

[0139] In an alternate approach, physical and/or chemical cross-linking methods may be applied to improve the bond strength between the polymeric coating containing the drugs, agents or compounds and the surface of the medical device or between the polymeric coating containing the drugs, agents or compounds and a primer. Alternately, other primers applied by either tra-

ditional coating methods such as dip, spray or spin coating, or by RF-plasma polymerisation may also be used to improve bond strength. For example, as shown in Figure 23, the bond strength can be improved by first depositing a primer layer 700 such as vapour polymerised parylene-C on the device surface, and then placing a secondary layer 702 which comprises a polymer that is similar in chemical composition to the one or more of the polymers that make up the drug-containing matrix 704, e.g., polyethylene-co-vinyl acetate or polybutyl methacrylate but has been modified to contain cross-linking moieties. This secondary layer 702 is then cross-linked to the primer after exposure to ultra-violet light. It should be noted that anyone familiar with the art would recognise that a similar outcome could be achieved using cross-linking agents that are activated by heat with or without the presence of an activating agent. The drug-containing matrix 704 is then layered onto the secondary layer 702 using a solvent that swells, in part or wholly, the secondary layer 702. This promotes the entrapment of polymer chains from the matrix into the secondary layer 702 and conversely from the secondary layer 702 into the drug-containing matrix 704. Upon removal of the solvent from the coated layers, an interpenetrating or interlocking network of the polymer chains is formed between the layers thereby increasing the adhesion strength between them. A top coat 706 is used as described above.

[0140] A related difficulty occurs in medical devices such as stents. In the drug-coated stents crimped state, some struts come into contact with each other and when the stent is expanded, the motion causes the polymeric coating comprising the drugs, agents or compounds to stick and stretch. This action may potentially cause the coating to separate from the stent in certain areas. The predominant mechanism of the coating self-adhesion is believed to be due to mechanical forces. When the polymer comes in contact with itself, its chains can tangle causing the mechanical bond, similar to Velcro®. Certain polymers do not bond with each other, for example, fluoropolymers. For other polymers, however, powders may be utilised. In other words, a powder may be applied to the one or more polymers incorporating the drugs, agents or other compounds on the surfaces of the medical device to reduce the mechanical bond. Any suitable biocompatible material which does not interfere with the drugs, agents, compounds or materials utilised to immobilise the drugs, agents or compounds onto the medical device may be utilised. For example, a dusting with a water soluble powder may reduce the tackiness of the coatings surface and this will prevent the polymer from sticking to itself thereby reducing the potential for delamination. The powder should be water-soluble so that it does not present an emboli risk. The powder may comprise an anti-oxidant, such as vitamin C, or it may comprise an anti-coagulant, such as aspirin or heparin. An advantage of utilizing an anti-oxidant may be in the fact that the anti-oxidant may preserve the other drugs,

agents or compounds over longer periods of time.

[0141] It is important to note that crystalline polymers are generally not sticky or tacky. Accordingly, if crystalline polymers are utilised rather than amorphous polymers, then additional materials may not be necessary. It is also important to note that polymeric coatings without drugs, agents and/or compounds may improve the operating characteristics of the medical device. For example, the mechanical properties of the medical device may be improved by a polymeric coating, with or without drugs, agents and/or compounds. A coated stent may have improved flexibility and increased durability. In addition, the polymeric coating may substantially reduce or eliminate galvanic corrosion between the different metals comprising the medical device. The same holds true for anastomosis devices.

[0142] Any of the above-described medical devices may be utilised for the local delivery of drugs, agents and/or compounds to other areas, not immediately around the device itself. In order to avoid the potential complications associated with systemic drug delivery, the medical devices of the present invention may be utilised to deliver therapeutic agents to areas adjacent to the medical device. For example, a rapamycin coated stent may deliver the rapamycin to the tissues surrounding the stent as well as areas upstream of the stent and downstream of the stent. The degree of tissue penetration depends on a number of factors, including the drug, agent or compound, the concentrations of the drug and the release rate of the agent. The same holds true for coated anastomosis devices.

[0143] The drug, agent and/or compound/carrier or vehicle compositions described above may be formulated in a number of ways. For example, they may be formulated utilizing additional components or constituents, including a variety of excipient agents and/or formulary components to affect ease of manufacture, coating integrity, ease of sterilisation, drug stability, and drug release rate. Within exemplary embodiments of the present invention, excipient agents and/or formulary components may be added to achieve both fast-release and sustained-release drug elution profiles. Such excipient agents may include salts and/or inorganic compounds such as acids/bases or buffer components, antioxidants, surfactants, polypeptides, proteins, carbohydrates including sucrose, glucose or dextrose, chelating agents such as EDTA, glutathione or other excipients or agents.

[0144] It is important to note that any of the above-described medical devices may be coated with coatings that comprise drugs, agents or compounds or simply with coatings that contain no drugs, agents or compounds. In addition, the entire medical device may be coated or only a portion of the device may be coated. The coating may be uniform or nonuniform. The coating may be discontinuous.

[0145] As described above, any number of drugs, agents and/or compounds may be locally delivered via

any number of medical devices. For example, stents and anastomosis devices may incorporate coatings comprising drugs, agents and/or compounds to treat various disease states and reactions by the body as described in detail above. Other devices which may be coated with or otherwise incorporate therapeutic dosages of drugs, agents and/or compounds include stent-grafts, which are briefly described above, and devices utilizing stent-grafts, such as devices for treating abdominal aortic aneurysms as well as other aneurysms, e.g. thoracic aorta aneurysms.

[0146] Stent-grafts, as the name implies, comprise a stent and a graft material attached thereto. Figure 24 illustrates an exemplary stent-graft 800. The stent-graft 800 may comprise any type of stent and any type of graft material as described in detail subsequently. In the illustrated exemplary embodiment, the stent 802 is a self-expanding device. A typical self-expanding stent comprises an expandable lattice or network of interconnected struts. In preferred embodiments of the invention, the lattice is fabricated, e.g. laser cut, from an integral tube of material.

[0147] In accordance with the present invention, the stent may be variously configured. For example, the stent may be configured with struts or the like that form repeating geometric shapes. One skilled in the art will readily recognise that a stent may be configured or adapted to include certain features and/or to perform a certain function(s), and that alternate designs may be used to promote that feature or function.

[0148] In the exemplary embodiment of the invention illustrated in Figure 24, the matrix or struts of stent 802 may be configured into at least two hoops 804, each hoop 804 comprising a number of struts 806 formed into a diamond shape, having approximately nine diamonds. The stent 802 may further include a zigzag shaped ring 808 for connecting adjacent hoops to one another. The zigzag shaped rings 808 may be formed from a number of alternating struts 810, wherein each ring has fifty-four struts.

[0149] An inner or outer surface of the stent 802 may be covered by or support a graft material. Graft material 812 may be made from any number of materials known to those skilled in the art, including woven polyester, Dacron®, Teflon®, polyurethane porous polyurethane, silicone, polyethylene, terephthalate, expanded polytetrafluoroethylene (ePTFE) and blends of various materials.

[0150] The graft material 812 may be variously configured, preferably to achieve predetermined mechanical properties. For example, the graft material may incorporate a single or multiple weaving and/or pleating patterns, or may be pleated or unpleated. For example, the graft material may be configured into a plain weave, a satin weave, include longitudinal pleats, interrupted pleats, annular or helical pleats, radially oriented pleats, or combinations thereof. Alternately, the graft material may be knitted or braided. In the embodiments of the

invention in which the graft material is pleated, the pleats may be continuous or discontinuous. Also, the pleats may be oriented longitudinally, circumferentially, or combinations thereof.

[0151] As illustrated in Figure 24, the graft material 812 may include a plurality of longitudinal pleats 814 extending along its surface, generally parallel to the longitudinal axis of the stent-graft 800. The pleats 814 allow the stent-graft 800 to collapse around its centre, much as it would be when it is delivered into a patient. This provides a relatively low profile delivery system, and provides for a controlled and consistent deployment therefrom. It is believed that this configuration minimises wrinkling and other geometric irregularities. Upon subsequent expansion, the stent-graft 800 assumes its natural cylindrical shape, and the pleats 814 uniformly and symmetrically open.

[0152] In addition, the pleats 814 help facilitate stent-graft manufacture, in that they indicate the direction parallel to the longitudinal axis, allowing stent to graft attachment along these lines, and thereby inhibiting accidental twisting of the graft relative to the stent after attachment. The force required to push the stent-graft 800 out of the delivery system may also be reduced, in that only the pleated edges of the graft make frictional contact with the inner surface of the delivery system. One further advantage of the pleats 814 is that blood tends to coagulate generally uniformly in the troughs of the pleats 814, discouraging asymmetric or large clot formation on the graft surface, thereby reducing embolus risk.

[0153] As shown in Figure 24, the graft material 812 may also include one or more, and preferably a plurality of, radially oriented pleat interruptions 816. The pleat interruptions 816 are typically substantially circular and are oriented perpendicular to longitudinal axis. Pleat interruptions 816 allow the graft and stent to bend better at selective points. This design provides for a graft material that has good crimpability and improved kink resistance.

[0154] The foregoing graft materials may be knitted or woven, and may be warp or weft knitted. If the material is warp knitted, it may be provided with a velour, or towel like surface, which is believed to speed the formation of blood clots, thereby promoting the integration of a stent-graft or stent-graft component into the surrounding cellular structure.

[0155] A graft material may be attached to a stent or to another graft material by any number of structures or methods known to those skilled in the art, including adhesives, such as polyurethane glue; a plurality of conventional sutures of polyvinylidene fluoride, polypropylene, polyester (such as that sold under the trade mark Dacron), or any other suitable material; ultrasonic welding; mechanical interference fit; and staples.

[0156] The stent 802 and/or graft material 812 may be coated with any of the above-described drugs, agents and/or compounds. In one exemplary embodi-

ment, rapamycin may be affixed to at least a portion of the graft material 812 utilizing any of the materials and processes described above. In another exemplary embodiment, rapamycin may be affixed to at least a portion of the graft material 812 and heparin or other antithrombotics may be affixed to at least a portion of the stent 802. With this configuration, the rapamycin coated graft material 812 may be utilised to minimise or substantially eliminate smooth muscle cell hyperproliferation and the heparin coated stent may substantially reduce the chance of thrombosis.

[0157] The particular polymer(s) utilised depends on the particular material upon which it is affixed. In addition, the particular drug, agent and/or compound may also affect the selection of polymer(s). As set forth above, rapamycin may be affixed to at least a portion of the graft material 812 utilizing the polymer(s) and processes described above. In another alternate exemplary embodiment, the rapamycin or any other drug, agent and/or compound may be directly impregnated into the graft material 812 utilizing any number of known techniques.

[0158] In yet another alternate exemplary embodiment, the stent-graft may be formed from two stents with the graft material sandwiched between them. Figure 25 is a simple illustration of a stent-graft 900 formed from an inner stent 902, an outer stent 904 and graft material 906 sandwiched between them. The stents 902, 904 and graft material 906 may be formed from the same materials as described above. As before, the inner stent 902 may be coated with an antithrombotic or anticoagulant such as heparin while the outer stent 904 may be coated with an antiproliferative such as rapamycin. Alternately, the graft material 906 may be coated with any of the above described drugs, agents and/or compounds, as well as combinations thereof, or all three elements may be coated with the same or different drugs, agents and/or compounds.

[0159] In yet another alternate exemplary embodiment, the stent-graft design may be modified to include a graft cuff. As illustrated in Figure 26, the graft material 906 may be folded around the outer stent 904 to form cuffs 908. In this exemplary embodiment, the cuffs 908 may be loaded with various drugs, agents and/or compounds, including rapamycin and heparin. The drugs, agents and/or compounds may be affixed to the cuffs 908 utilizing the methods and materials described above or through other means. For example, the drugs, agents and/or compounds may be trapped in the cuffs 908 with the graft material 906 acting as the diffusion barrier through which the drug, agent and/or compound elutes. The particular material selected as well as its physical characteristics would determine the elution rate. Alternately, the graft material 906 forming the cuffs 908 may be coated with one or more polymers to control the elution rate as described above.

[0160] Stent-grafts may be utilised to treat aneurysms. An aneurysm is an abnormal dilation of a layer

or layers of an arterial wall, usually caused by a systemic collagen synthetic or structural defect. An abdominal aortic aneurysm is an aneurysm in the abdominal portion of the aorta, usually located in or near one or both of the two iliac arteries or near the renal arteries. The aneurysm often arises in the infrarenal portion of the diseased aorta, for example, below the kidneys. A thoracic aortic aneurysm is an aneurysm in the thoracic portion of the aorta. When left untreated, the aneurysm may rupture, usually causing rapid fatal haemorrhaging.

[0161] Aneurysms may be classified or typed by their position as well as by the number of aneurysms in a cluster. Typically, abdominal aortic aneurysms may be classified into five types. A Type I aneurysm is a single dilation located between the renal arteries and the iliac arteries. Typically, in a Type I aneurysm, the aorta is healthy between the renal arteries and the aneurysm and between the aneurysm and the iliac arteries.

[0162] A Type II A aneurysm is a single dilation located between the renal arteries and the iliac arteries. In a Type II A aneurysm, the aorta is healthy between the renal arteries and the aneurysm, but not healthy between the aneurysm and the iliac arteries. In other words, the dilation extends to the aortic bifurcation. A Type II B aneurysm comprises three dilations. One dilation is located between the renal arteries and the iliac arteries. Like a Type II A aneurysm, the aorta is healthy between the aneurysm and the renal arteries, but not healthy between the aneurysm and the iliac arteries. The other two dilations are located in the iliac arteries between the aortic bifurcation and the bifurcations between the external iliacs and the internal iliacs. The iliac arteries are healthy between the iliac bifurcation and the aneurysms. A Type II C aneurysm also comprises three dilations. However, in a Type II C aneurysm, the dilations in the iliac arteries extend to the iliac bifurcation.

[0163] A Type III aneurysm is a single dilation located between the renal arteries and the iliac arteries. In a Type III aneurysm, the aorta is not healthy between the renal arteries and the aneurysm. In other words, the dilation extends to the renal arteries.

[0164] A ruptured abdominal aortic aneurysm is presently the thirteenth leading cause of death in the United States. The routine management of abdominal aortic aneurysms has been surgical bypass, with the placement of a graft in the involved or dilated segment. Although resection with a synthetic graft via transperitoneal or retroperitoneal approach has been the standard treatment, it is associated with significant risk. For example, complications include perioperative myocardial ischemia, renal failure, erectile impotence, intestinal ischemia, infection, lower limb ischemia, spinal cord injury with paralysis, aorta-enteric fistula, and death. Surgical treatment of abdominal aortic aneurysms is associated with an overall mortality rate of five percent in asymptomatic patients, sixteen to nineteen percent in symptomatic patients, and is as high as fifty percent in patients with ruptured abdominal aortic aneurysms.

[0165] Disadvantages associated with conventional surgery, in addition to the high mortality rate, include an extended recovery period associated with the large surgical incision and the opening of the abdominal cavity, difficulties in suturing the graft to the aorta, the loss of the existing thrombosis to support and reinforce the graft, the unsuitability of the surgery for many patients having abdominal aortic aneurysms, and the problems associated with performing the surgery on an emergency basis after the aneurysm has ruptured. Further, the typical recovery period is from one to two weeks in the hospital, and a convalescence period at home from two to three months or more, if complications ensue. Since many patients having abdominal aortic aneurysms have other chronic illnesses, such as heart, lung, liver and/or kidney disease, coupled with the fact that many of these patients are older, they are less than ideal candidates for surgery.

[0166] The occurrence of aneurysms is not confined to the abdominal region. While abdominal aortic aneurysms are generally the most common, aneurysms in other regions of the aorta or one of its branches are possible. For example, aneurysms may occur in the thoracic aorta. As is the case with abdominal aortic aneurysms, the widely accepted approach to treating an aneurysm in the thoracic aorta is surgical repair, involving replacing the aneurysmal segment with a prosthetic device. This surgery, as described above, is a major undertaking, with associated high risks and with significant mortality and morbidity.

[0167] Over the past five years, there has been a great deal of research directed at developing less invasive, percutaneous, e.g., catheter directed, techniques for the treatment of aneurysms, specifically abdominal aortic aneurysms. This has been facilitated by the development of vascular stents, which can and have been used in conjunction with standard or thin-wall graft material in order to create a stent-graft or endograft. The potential advantages of less invasive treatments have included reduced surgical morbidity and mortality along with shorter hospital and intensive care unit stays.

[0168] Stent-grafts or endoprostheses are now FDA approved and commercially available. The delivery procedure typically involves advanced angiographic techniques performed through vascular accesses gained via surgical cutdown of a remote artery, such as the common femoral or brachial arteries. Over a guidewire, the appropriate size introducer will be placed. The catheter and guidewire are passed through the aneurysm, and, with the appropriate size introducer housing a stent-graft, the stent-graft will be advanced along the guidewire to the appropriate position. Typical deployment of the stent-graft device requires withdrawal of an outer sheath while maintaining the position of the stent-graft with an inner-stabilizing device. Most stent-grafts are self-expanding; however, an additional angioplasty procedure, e.g., balloon angioplasty, may be required to secure the position of the stent-graft. Following the

placement of the stent-graft, standard angiographic views may be obtained.

[0169] Due to the large diameter of the above-described devices, typically greater than twenty French (3F = 1mm), arteriotomy closure requires surgical repair. Some procedures may require additional surgical techniques, such as hypogastric artery embolisation, vessel ligation, or surgical bypass, in order to adequately treat the aneurysm or to maintain flow to both lower extremities. Likewise, some procedures will require additional, advanced catheter directed techniques, such as angioplasty, stent placement, and embolisation, in order to successfully exclude the aneurysm and efficiently manage leaks.

[0170] While the above-described endoprostheses represent a significant improvement over conventional surgical techniques, there is a need to improve the endoprostheses, their method of use and their applicability to varied biological conditions. Accordingly, in order to provide a safe and effective alternate means for treating aneurysms, including abdominal aortic aneurysms and thoracic aortic aneurysms, a number of difficulties associated with currently known endoprostheses and their delivery systems must be overcome. One concern with the use of endoprostheses is the prevention of endoleaks and the disruption of the normal fluid dynamics of the vasculature. Devices using any technology should preferably be simple to position and reposition as necessary, should preferably provide an acute fluid tight seal, and should preferably be anchored to prevent migration without interfering with normal blood flow in both the aneurysmal vessel as well as branching vessels. In addition, devices using the technology should preferably be able to be anchored, sealed, and maintained in bifurcated vessels, tortuous vessels, highly angulated vessels, partially diseased vessels, calcified vessels, odd shaped vessels, short vessels, and long vessels. In order to accomplish this, the endoprostheses should preferably be extendable and re-configurable while maintaining acute and long term fluid tight seals and anchoring positions.

[0171] The endoprostheses should also preferably be able to be delivered percutaneously utilizing catheters, guidewires and other devices which substantially eliminate the need for open surgical intervention. Accordingly, the diameter of the endoprostheses in the catheter is an important factor. This is especially true for aneurysms in the larger vessels, such as the thoracic aorta.

[0172] As stated above, one or more stent-grafts may be utilized to treat aneurysms. These stent-grafts or endoprostheses may comprise any number of materials and configurations. Figure 23 illustrates an exemplary system for treating abdominal aortic aneurysms. The system 1000 includes a first prosthesis 1002 and two second prostheses 1004 and 1006, which in combination, bypass an aneurysm 1008. In the illustrated exemplary embodiment, a proximal portion of the system 1000 may be positioned in a section 1010 of an artery

upstream of the aneurysm 1008, and a distal portion of the system 1000 may be positioned in a downstream section of the artery or a different artery such as iliacs 1012 and 1014.

[0173] A prosthesis used in a system in accordance with the present invention typically includes a support, stent or lattice of interconnected struts defining an interior space or lumen having an open proximal end and an open distal end. The lattice also defines an interior surface and an exterior surface. The interior and/or exterior surfaces of the lattice, or a portion of the lattice, may be covered by or support at least one gasket material or graft material.

[0174] In preferred embodiments of the invention, a prosthesis is moveable between an expanded or inflated position and an unexpanded or deflated position, and any position between them. In some exemplary embodiments of the invention, it may be desirable to provide a prosthesis that moves only from fully collapsed to fully expanded. In other exemplary embodiments of the invention, it may be desirable to expand the prosthesis, then collapse or partially collapse the prosthesis. Such capability is beneficial to the surgeon to properly position or re-position the prosthesis. In accordance with the present invention, the prosthesis may be self-expanding, or may be expandable using an inflatable device, such as a balloon or the like.

[0175] Referring back to Figure 27, the system 1000 is deployed in the infrarenal neck 1010 of the abdominal aorta, upstream of where the artery splits into first and second common iliac arteries 1012, 1014. Figure 27 shows the first prosthesis or stent gasket 1002 positioned in the infrarenal neck 1010; two second prostheses, 1004, 1006, the proximal ends of which matingly engage a proximal portion of stent gasket 1002, and the distal ends of which extend into a common iliac artery 1012 or 1014. As illustrated, the body of each second prosthesis forms a conduit or fluid flow path that passes through the location of the aneurysm 1008. In preferred embodiments of the invention, the components of the system 1000 define a fluid flow path that bypasses the section of the artery where the aneurysm is located.

[0176] The first prosthesis includes a support matrix or stent that supports a sealing material or foam, at least a portion of which is positioned across a biological fluid flow path, e.g., across a blood flow path. In preferred embodiments of the invention, the first prosthesis, the stent, and the sealing material are radially expandable, and define a hollow space between a proximal portion of the prosthesis and a distal portion of the prosthesis. The first prosthesis may also include one or more structures for positioning and anchoring the prosthesis in the artery, and one or more structures for engaging and fixing at least one second prosthesis in place, e.g., a bypass prosthesis.

[0177] The support matrix or stent of the first prosthesis may be formed of a wide variety of materials, may be configured in a wide variety of shapes, and their

shapes and uses are well known in the art. Exemplary prior art stents are disclosed in US-4733665, US-4739762 and US-4776337.

[0178] In preferred embodiments of the invention, the stent of the first prosthesis is a collapsible, flexible, and self-expanding lattice or matrix formed from a metal or metal alloy, such as a nickel titanium based shape memory alloy (for example nitinol) or stainless steel. Structures formed from stainless steel may be made self-expanding by configuring the stainless steel in a predetermined manner, for example, by twisting it into a braided configuration. More preferably, the stent is a tubular frame that supports a sealing material. The term tubular, as used herein, refers to any shape having a sidewall or sidewalls defining a hollow space or lumen extending between them; the cross-sectional shape may be generally cylindrical, elliptic, oval, rectangular, triangular, or any other shape. Furthermore, the shape may change or be deformable as a consequence of various forces that may press against the stent or prosthesis.

[0179] The sealing material or gasket member supported by the stent may be formed of a wide variety of materials, may be configured in a wide variety of shapes, and their shapes and uses are well known in the art. Exemplary materials for use with this aspect of the invention are disclosed in US-4739762 and US-4776337.

[0180] The sealing material or gasket member may comprise any suitable material. Exemplary materials preferably comprise a biodegradable and biocompatible material, including but are not limited to, open cell foam materials and closed cell foam materials. Exemplary materials include polyurethane, polyethylene, polytetrafluoroethylene; and other various polymer materials, preferably woven or knitted, that provide a flexible structure, such as a polyester, for example as sold under the trade mark Dacron. Highly compressible foams are particularly preferred, preferably to keep the crimped profile low for better delivery. The sealing material or foam is preferably substantially impervious to blood when in a compressed state.

[0181] The sealing material may cover one or more surfaces of the stent i.e., may be located along an interior or exterior wall, or both, and preferably extends across the proximal end or a proximal portion of the stent. The sealing material helps impede any blood trying to flow around the first prosthesis, e.g., between the first prosthesis and the arterial wall, and around one or more bypass prostheses after they have been deployed within the lumen of the first prosthesis (described in more detail below).

[0182] In preferred embodiments of the invention, the sealing material stretches or covers a portion of the proximal end of the stent and along at least a portion of the outside wall of the stent.

[0183] In some embodiments of the invention, it may be desirable for the portion of the sealing material covering the proximal portion of the stent to include one or

more holes, apertures, points, slits, sleeves, flaps, weakened spots, guides, or the like for positioning a guidewire, for positioning a system component, such as a second prosthesis, and/or for engaging, preferably matingly engaging, one or more system components, such as a second prosthesis. For example, a sealing material configured as a cover or the like, and having a hole, may partially occlude the stent lumen.

[0184] These openings may be variously configured, primarily to conform to its use. These structures promote proper side by side placement of one or more, preferably multiple, prostheses within the first prosthesis, and, in some embodiments of the invention, the sealing material may be configured or adapted to assist in maintaining a certain shape of the fully deployed system or component. Further, these openings may exist prior to deployment of the prosthesis, or may be formed in the prosthesis as part of a deployment procedure. The various functions of the openings will be evident from the description below. In exemplary embodiments of the invention, the sealing material is a foam cover that has a single hole.

[0185] The sealing material may be attached to the stent by any of a variety of connectors, including a plurality of conventional sutures of polyvinylidene fluoride, polypropylene, polyester, or any other suitable material and attached thereto. Other methods of attaching the sealing material to the stent include adhesives, ultrasonic welding, mechanical interference fit and staples.

[0186] One or more markers may be optionally disposed in or on the stent between the proximal end and the distal end. Preferably, two or more markers are sized and/or positioned to identify a location on the prosthesis, or to identify the position of the prosthesis, or a portion thereof, in relation to an anatomical feature or another system component.

[0187] A first prosthesis is typically deployed in an arterial passageway upstream of an aneurysm, and functions to open and/or expand the artery, to properly position and anchor the various components of the system, and, in combination with other components, seal the system or portions thereof from fluid leaks. For example, the sealing prosthesis may be deployed within the infrarenal neck, between an abdominal aortic aneurysm and the renal arteries of a patient, to assist in repairing an abdominal aortic aneurysm.

[0188] Figures 27-29 show an exemplary sealing prosthesis of the present invention. Sealing prosthesis 1002 includes a cylindrical or oval self-expanding lattice, support, or stent 1016, typically made from a plurality of interconnected struts 1018. Stent 1016 defines an interior space or lumen 1020 having two open ends, a proximal end 1022 and a distal end 1024. One or more markers 1026 may be optionally disposed in or on the stent between the proximal end 1022 and the distal end 1024.

[0189] Stent 1016 may further include at least two but preferably eight (as shown in Figure 28) spaced apart longitudinal legs 1028. Preferably, there is a leg extend-

ing from each apex 1030 of diamonds formed by struts 1018. At least one leg, but preferably each leg, includes a flange 1032 adjacent its distal end which allows for the stent 1016 to be retrievable into its delivery apparatus after partial or nearly full deployment thereof so that it can be turned, or otherwise repositioned for proper alignment.

[0190] Figure 29 shows the sealing material 1034 covering the proximal end 1022 of stent gasket 1002. In the exemplary embodiment shown in Figure 29, sealing prosthesis 1002 includes a sealing material 1034 having a first opening or hole 1036 and a second opening or slit 1038. The gasket material covers at least a portion of the interior or exterior of the stent, and most preferably covers substantially all of the exterior of the stent. For example, gasket material 1034 may be configured to cover stent 1016 from the proximal end 1022 to the distal end 1024, but preferably not covering longitudinal legs 1028.

[0191] The sealing material 1034 helps impede any blood trying to flow around bypass prostheses 1004 and 1006 after they have been deployed (as shown in Figure 27) and from flowing around the stent gasket 1002 itself. For this embodiment, sealing material 1034 is a compressible member or gasket located along the exterior of the stent 1016 and at least a portion of the interior of the stent 1016.

[0192] The second prostheses 1004 and 1006 may comprise stent-grafts such as described with respect to Figure 24 and may be coated with any of the drugs, agents and/or compounds as described above. In other words, the stent and/or the graft material may be coated with any of the above-described drugs, agents and/or compounds utilizing any of the above-described polymers and processes. The stent gasket 1002 may also be coated with any of the above-described drugs, agents and/or compounds. In other words, the stent and/or sealing material may be coated with any of the above-described drugs, agents and/or compounds utilizing any of the above-described polymers and processes. In particular, rapamycin and heparin may be of importance to prevent smooth muscle cell hyperproliferation and thrombosis. Other drugs, agents and/or compounds may be utilised as well. For example drugs, agents and/or compounds which promote re-endothelialization may be utilised to facilitate incorporation of the prosthesis into the living organism. Also, embolic material may be incorporated into the stent-graft to reduce the likelihood of endo leaks.

[0193] It is important to note that the system which is described above for repairing abdominal aortic aneurysms is one example of such a system. Any number of aneurysmal repair systems comprising stent-grafts may be coated with the appropriate drugs, agents and/or compounds, as well as combinations thereof. For example, thoracic aorta aneurysms may be repaired in a similar manner. Regardless of the type of aneurysm or its position within the living organism, the components

comprising the repair system may be coated with the appropriate drug, agent and/or compound as described above with respect to stent-grafts.

Claims

1. A stent-graft for implantation into a treatment site of a living organism, comprising:
 - a scaffold structure for maintaining luminal patency;
 - a graft material secured to at least a portion of the scaffold structure;
 - a biocompatible vehicle affixed to at least one of the scaffold structure and graft material; and
 - at least one agent in therapeutic dosages incorporated into the biocompatible vehicle for the treatment of a disease condition.
2. A stent-graft as claimed in claim 1, in which the scaffold structure comprises a stent.
3. A stent-graft as claimed in claim 2, in which the stent is a self-expanding stent.
4. A stent-graft as claimed in claim 2, in which the graft material comprises a polymeric material.
5. A stent-graft as claimed in claim 4, in which the graft material comprises pleats.
6. A stent-graft as claimed in claim 5, in which the biocompatible vehicle comprises a polymeric matrix.
7. A stent-graft as claimed in claim 6, in which the polymeric matrix comprises poly(ethylene-co-vinylacetate) and polybutylmethacrylate.
8. A stent-graft as claimed in claim 7, in which the polymeric matrix comprises first and second layers, the first layer making contact with at least a portion of at least one of the scaffold structure and graft material and comprising a solution of poly(ethylene-co-vinylacetate) and polybutylmethacrylate; and the second layer comprising polybutylmethacrylate.
9. A stent-graft as claimed in claim 8, in which the at least one agent is incorporated into the first layer.
10. A stent-graft as claimed in claim 6, in which the biocompatible vehicle comprises a polyfluoro copolymer comprising polymerised residue of a first moiety selected from the group consisting of vinylidene fluoride and tetrafluoroethylene, and polymerised

residue of a second moiety other than the first moiety and which is copolymerised with the first moiety, thereby producing the polyfluoro copolymer, in which the relative amounts of the polymerised residue of the first moiety and the polymerised residue of the second moiety are effective to produce the biocompatible vehicle with properties effective for use in coating implantable medical devices when the coated medical device is subjected to a predetermined maximum temperature, and a solvent in which the polyfluoro copolymer is substantially soluble.

11. A stent-graft as claimed in claim 10, in which the polyfluoro copolymer comprises from about 50 to about 92 wt-% of the polymerised residue of the first moiety copolymerised with from about 50 to about 8 wt-% of the polymerised residue of the second moiety, preferably from about 50 to about 85 wt-% of the polymerised residue of vinylidene fluoride copolymerised with from about 50 to about 15 wt-% of the polymerised residue of the second moiety, especially from about 55 to about 65 wt-% of the polymerised residue of the vinylidene fluoride copolymerised with from about 45 to about 35 wt-% of the polymerised residue of the second moiety.
12. A stent-graft as claimed in claim 10, in which the second moiety is selected from the group consisting of hexafluoropropylene, tetrafluoroethylene, vinylidene fluoride, 1-hydropentafluoropropylene, perfluoro (methyl vinyl ether), chlorotrifluoroethylene, pentafluoropropene, trifluoroethylene, hexafluoroacetone and hexafluoroisobutylene.
13. A stent-graft as claimed in claim 1, in which the at least one agent has at least one of the properties selected from anti-proliferative, anti-inflammatory and anti-coagulant.
14. A stent-graft as claimed in claim 1, in which the at least one agent at least one of rapamycin and heparin.
15. A stent-graft as claimed in claim 1, which includes first and second scaffold structures for maintaining luminal patency, in which the biocompatible vehicle is affixed to at least one of the scaffold structures.
16. A stent-graft as claimed in claim 15, in which the first and second scaffold structures comprise stents, preferably self-expanding stents.
17. A stent-graft as claimed in claim 15, further comprising cuffs formed by folding and securing at least one end of the graft material over an end of one of the first and second scaffold structures.
18. A stent-graft as claimed in claim 17, in which the at least one therapeutic agent is encapsulated within the cuffs.
19. A stent-graft as claimed in claim 1, in which the at least one therapeutic agent is impregnated into the graft material.
20. A system for bypassing an aneurysm, comprising:
 - at least one prosthesis for establishing a fluid flow path through an aneurysmal section of artery;
 - an anchoring element operatively associated with the at least one prosthesis for securing and sealing the at least one prosthesis upstream of the aneurysmal section of artery;
 - a biocompatible vehicle affixed to at least one of the anchoring element and the at least one prosthesis; and
 - at least one agent in therapeutic dosages incorporated into the biocompatible material for treatment of a disease condition.
21. A system as claimed in claim 20, in which the at least one prosthesis comprises a stent-graft, preferably as claimed in any one of claims 1 to 19.
22. A system as claimed in claim 20, in which the anchoring element comprises a scaffold structure at least partially covered with a gasket material substantially impervious to blood.
23. A system as claimed in claim 22, in which the at least one therapeutic agent is impregnated into the gasket material.

FIG. 1

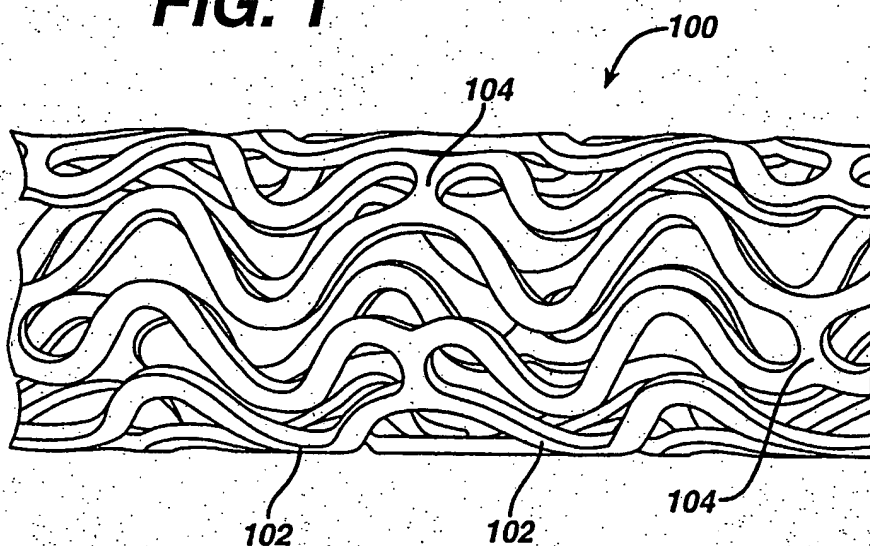


FIG. 2

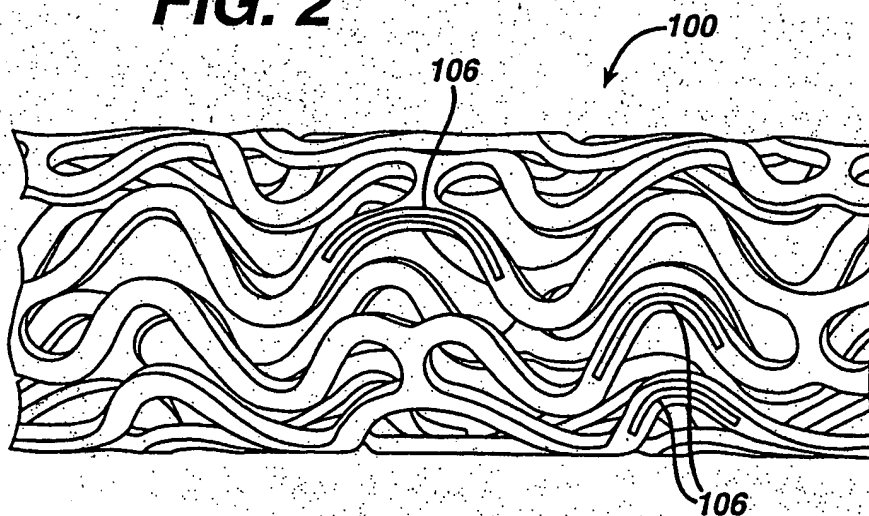


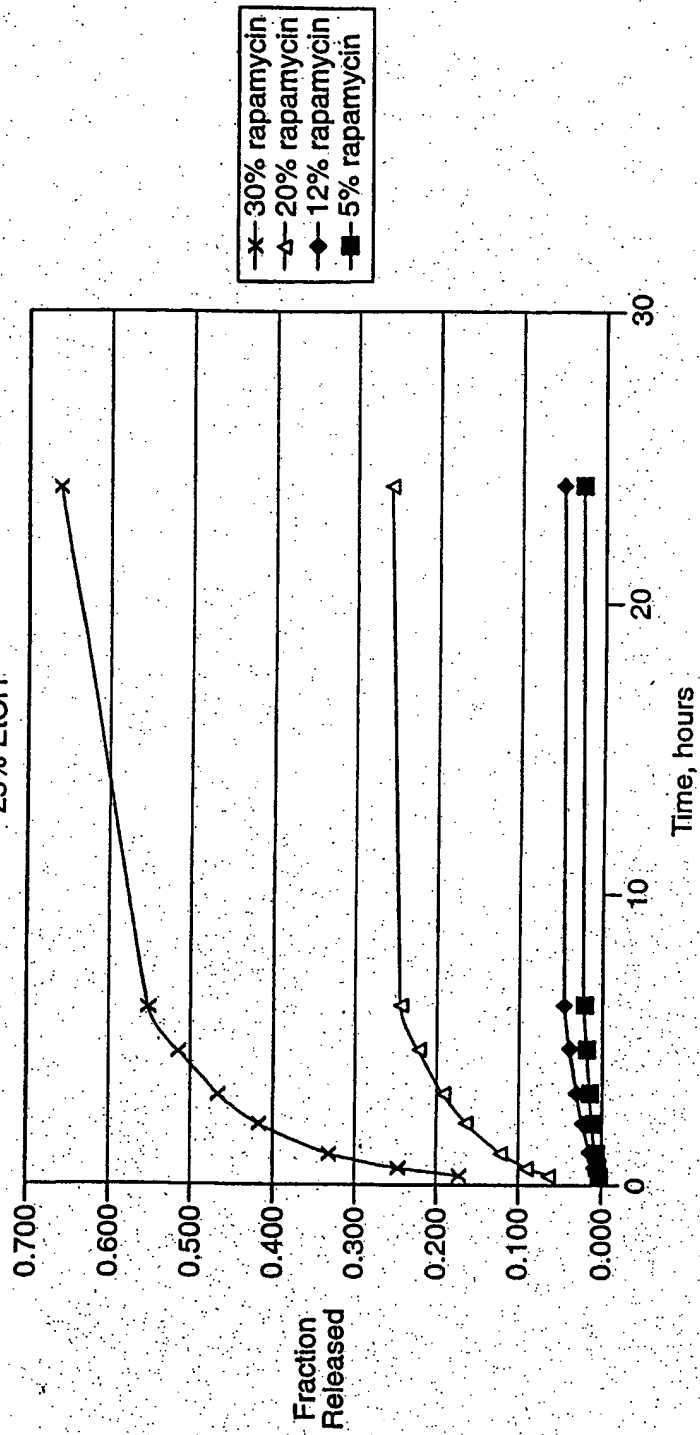
FIG. 3Rapamycin Release from VDF/HFP (84.5/14.5) in
25% EtOH

FIG. 4

Release in 25% Aq. Ethanol for
21508 + Rapamycin w/ top coat

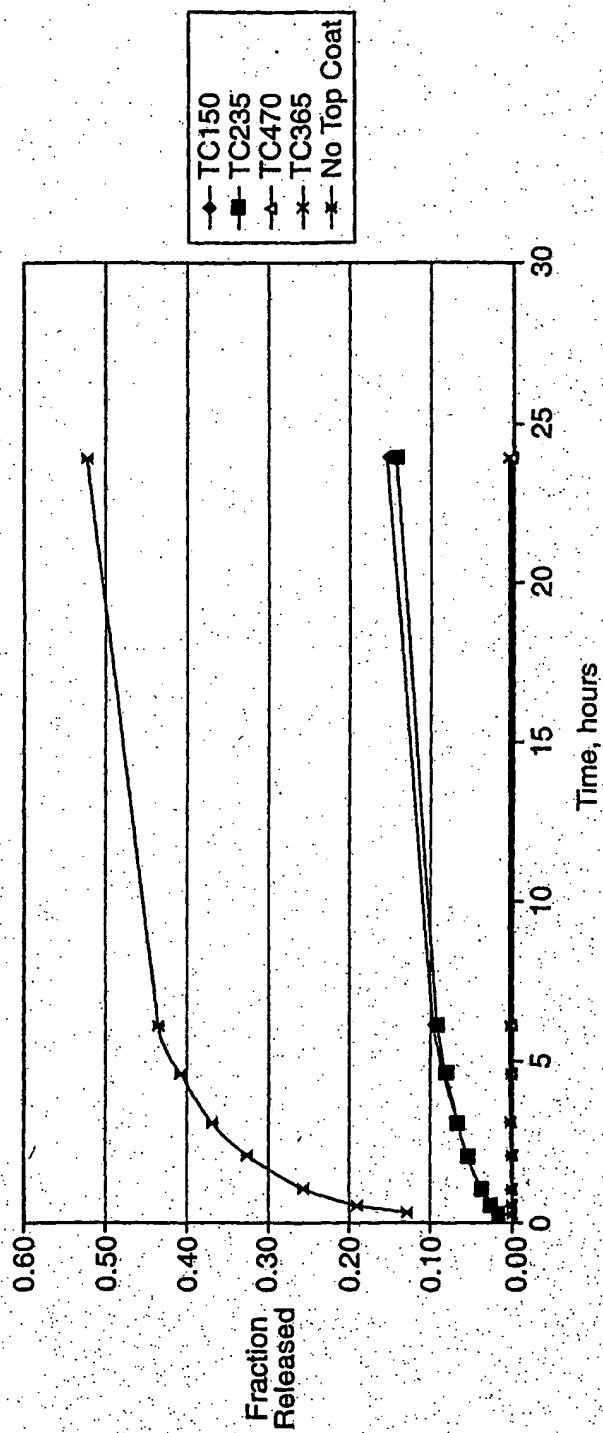


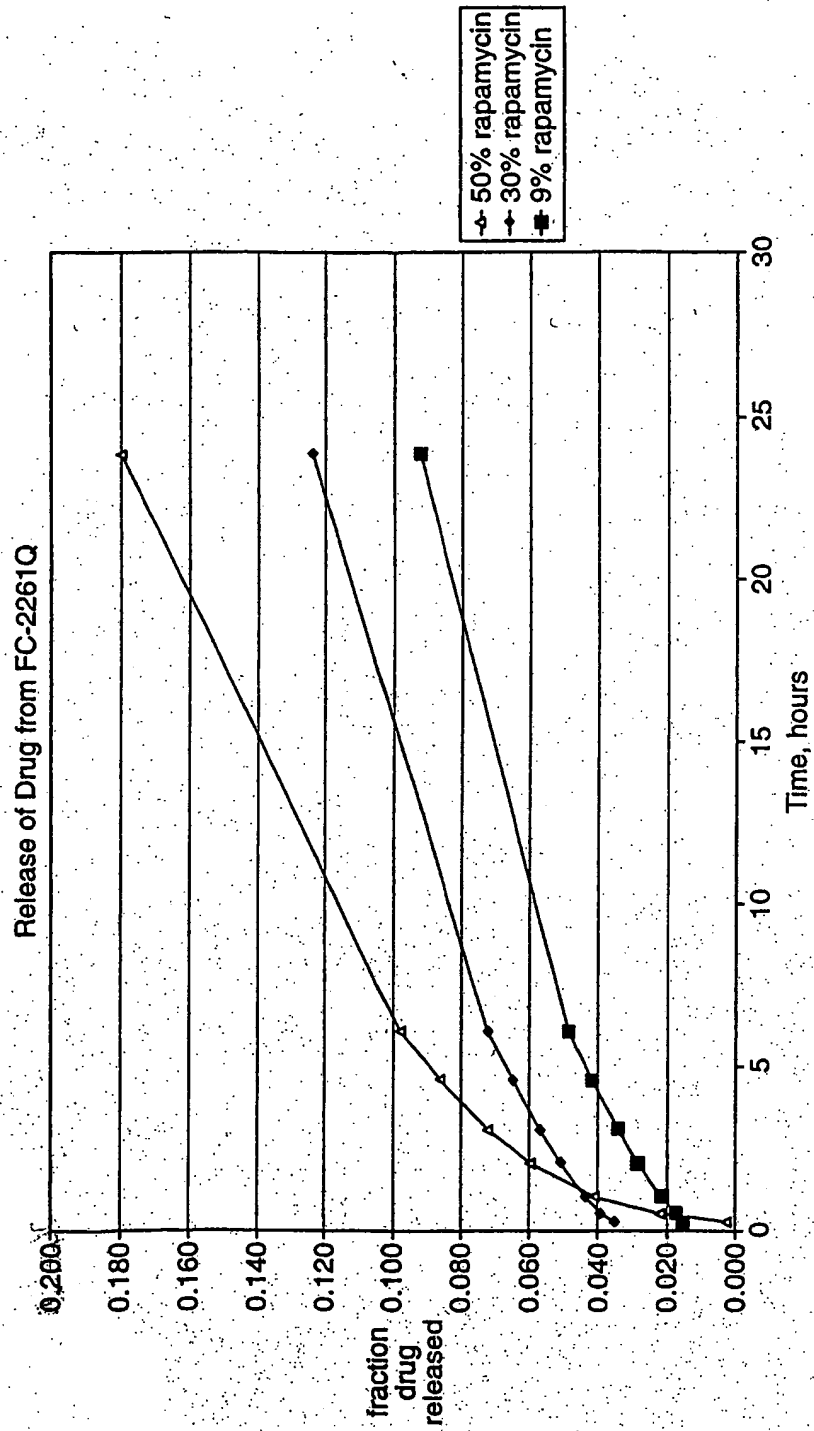
FIG. 5

FIG. 6

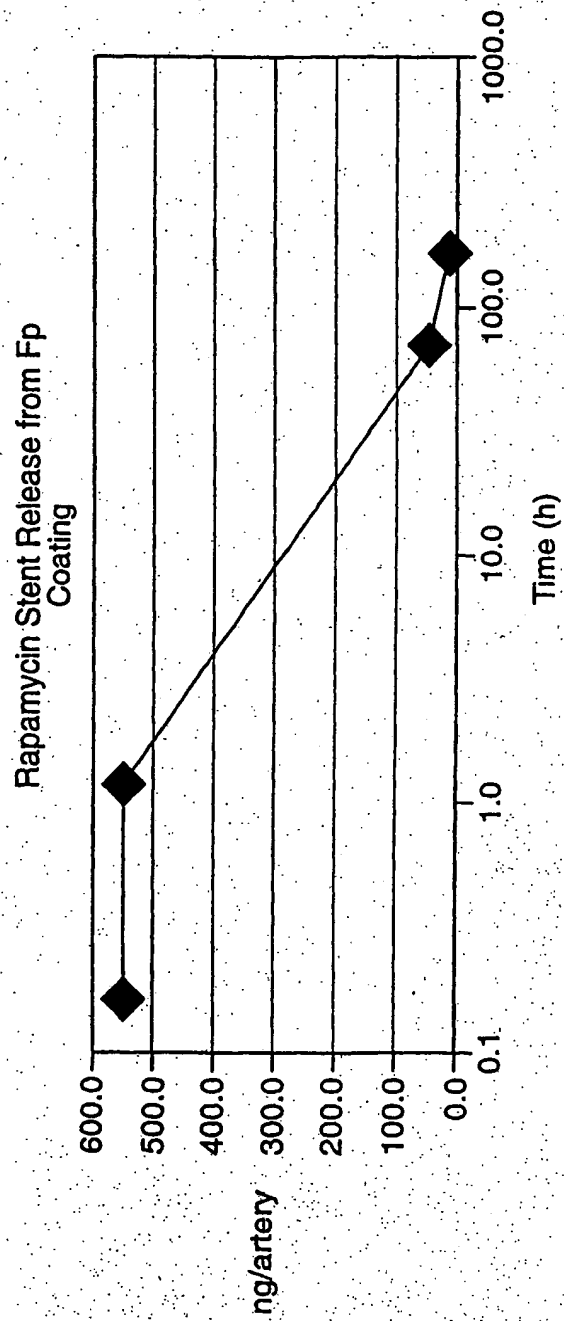


FIG. 7

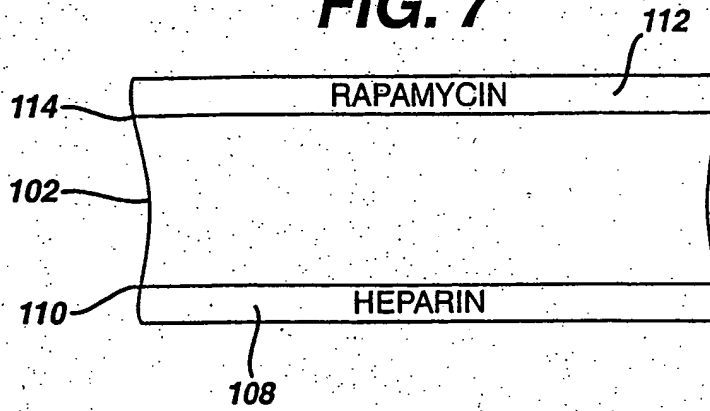


FIG. 8

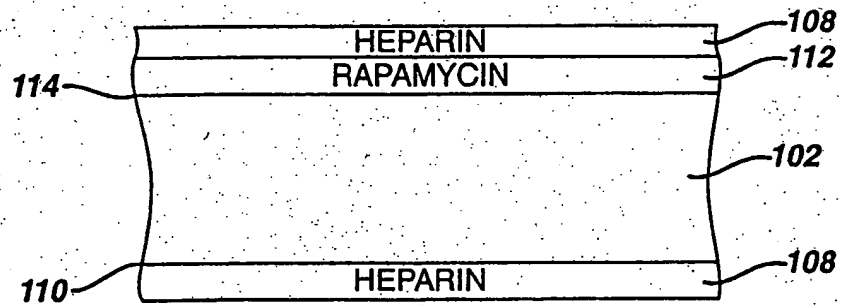


FIG. 9

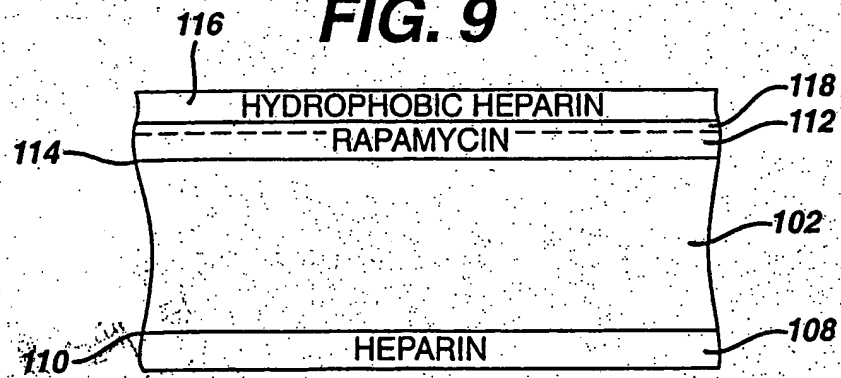


FIG. 10

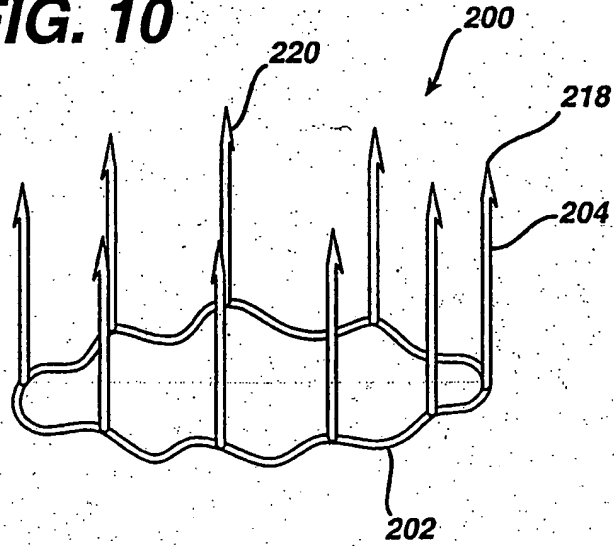


FIG. 11

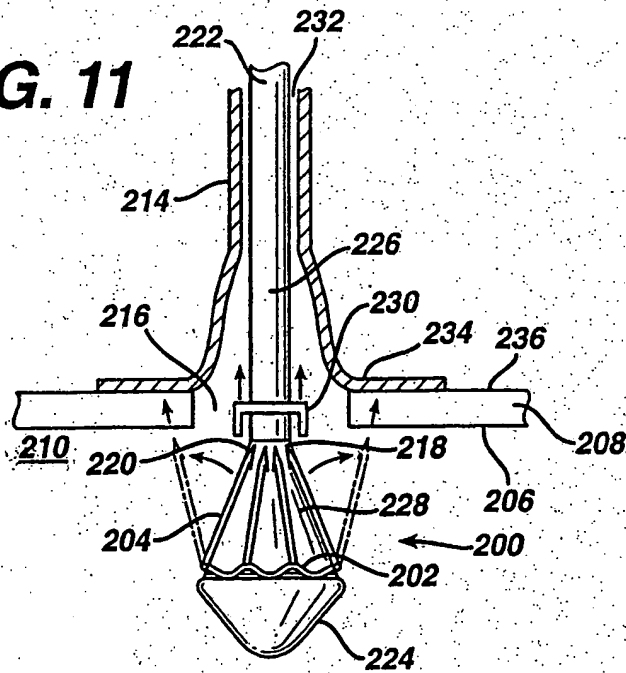


FIG. 12

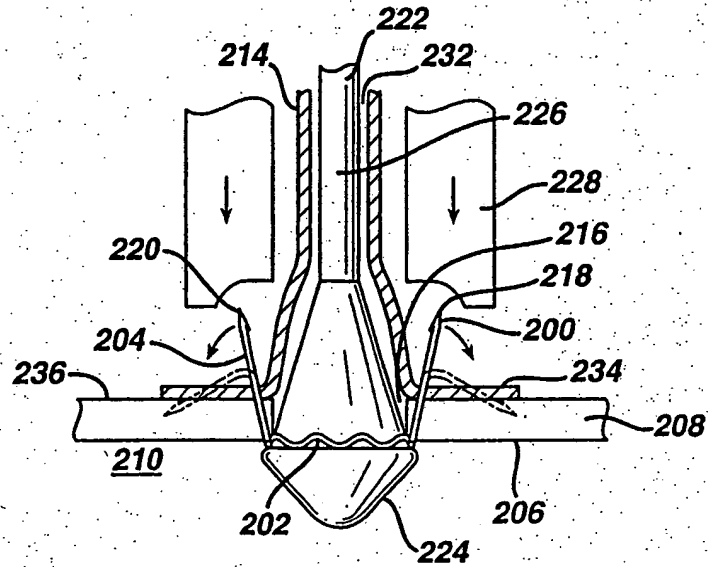


FIG. 13

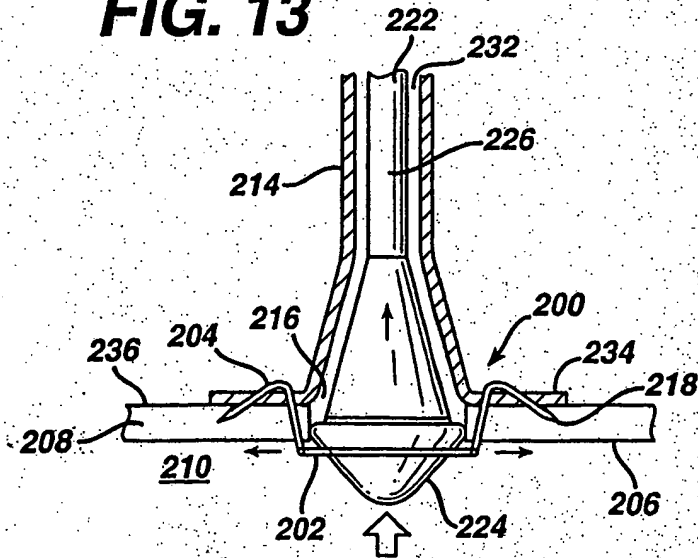


FIG. 14

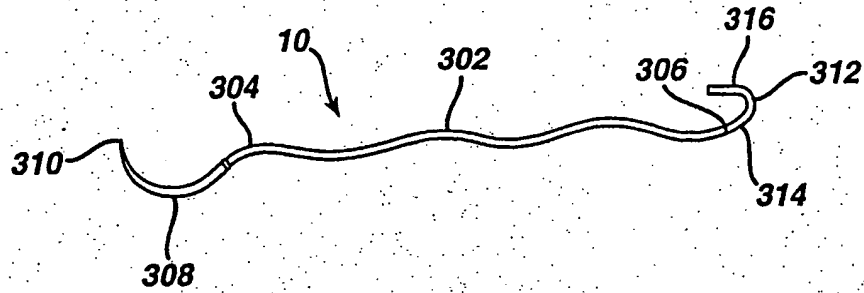


FIG. 15

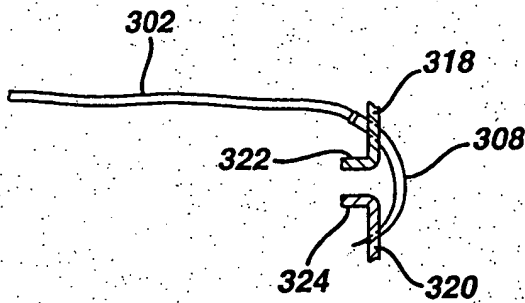


FIG. 16

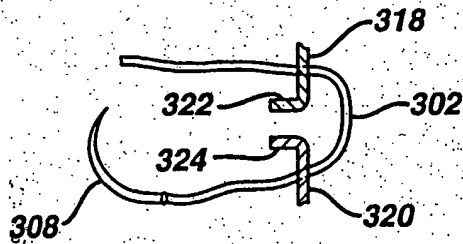


FIG. 17

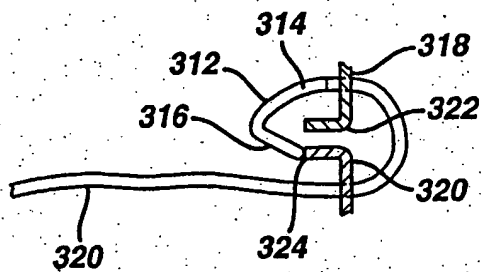


FIG. 18

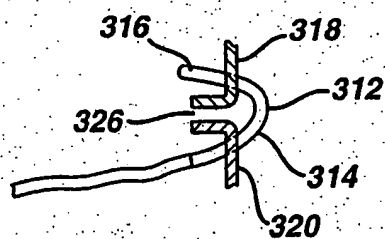


FIG. 19

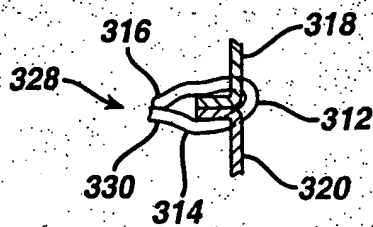


FIG. 20

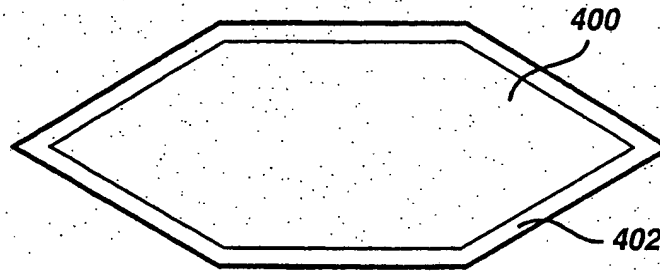


FIG. 21

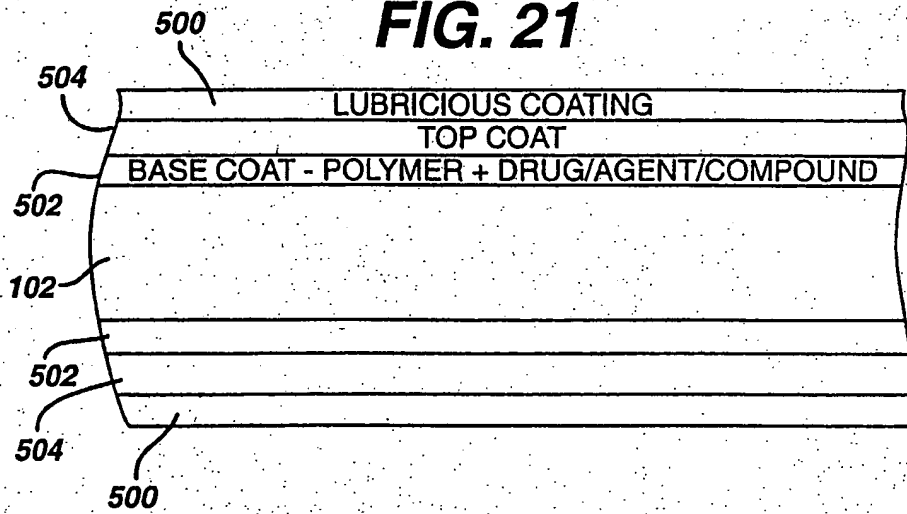


FIG. 22

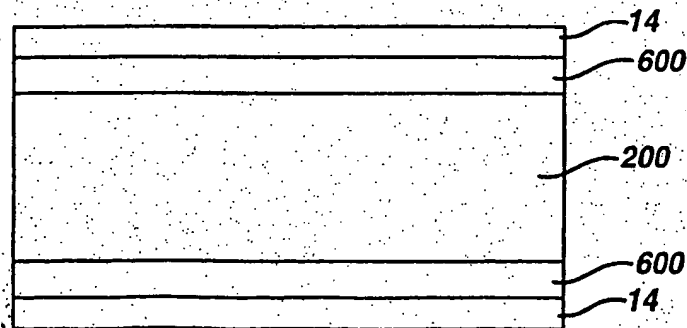


FIG. 23

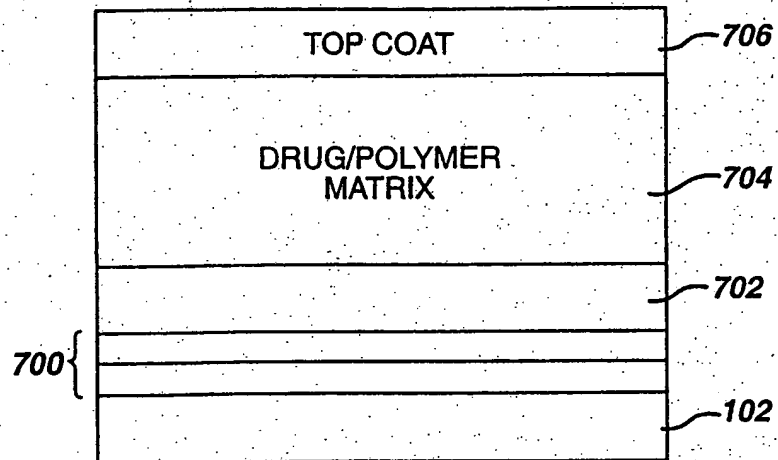


FIG. 24

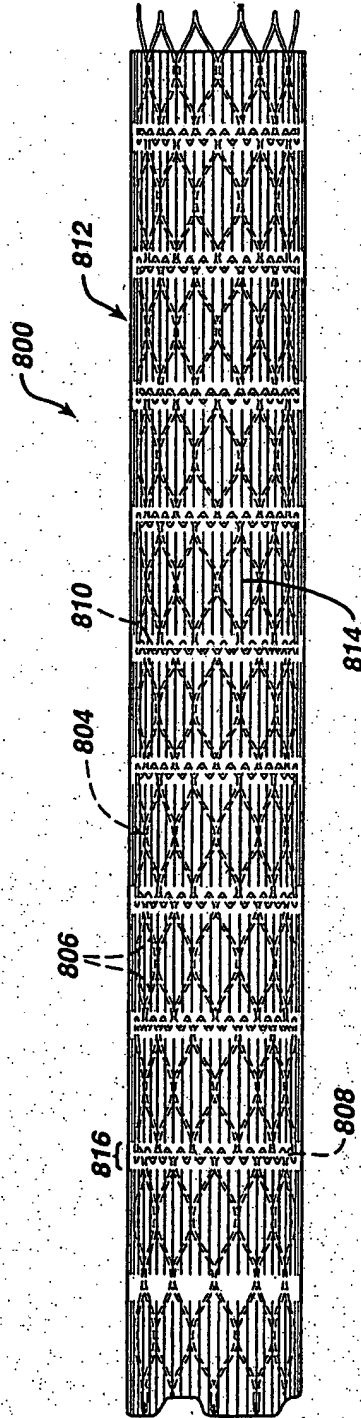


FIG. 25

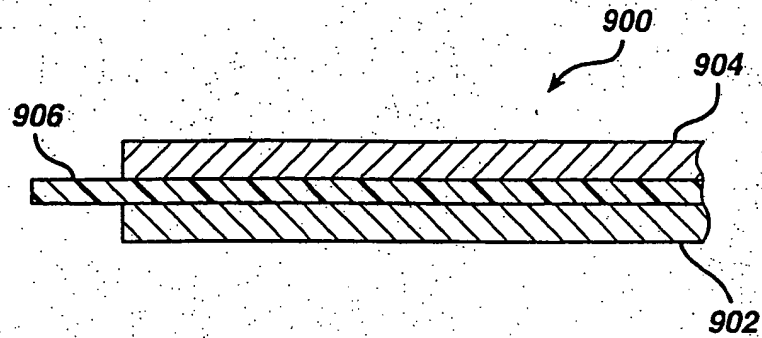
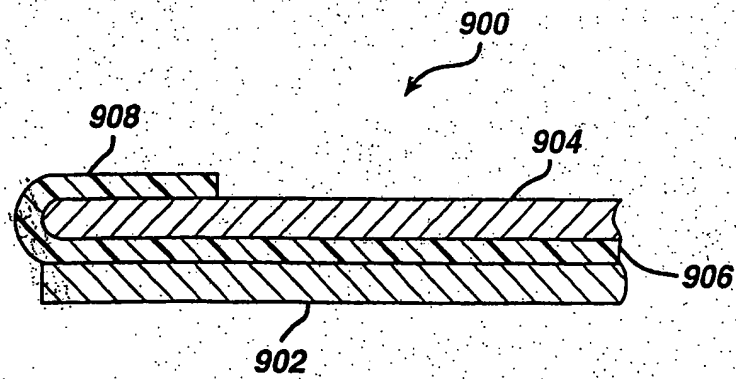


FIG. 26



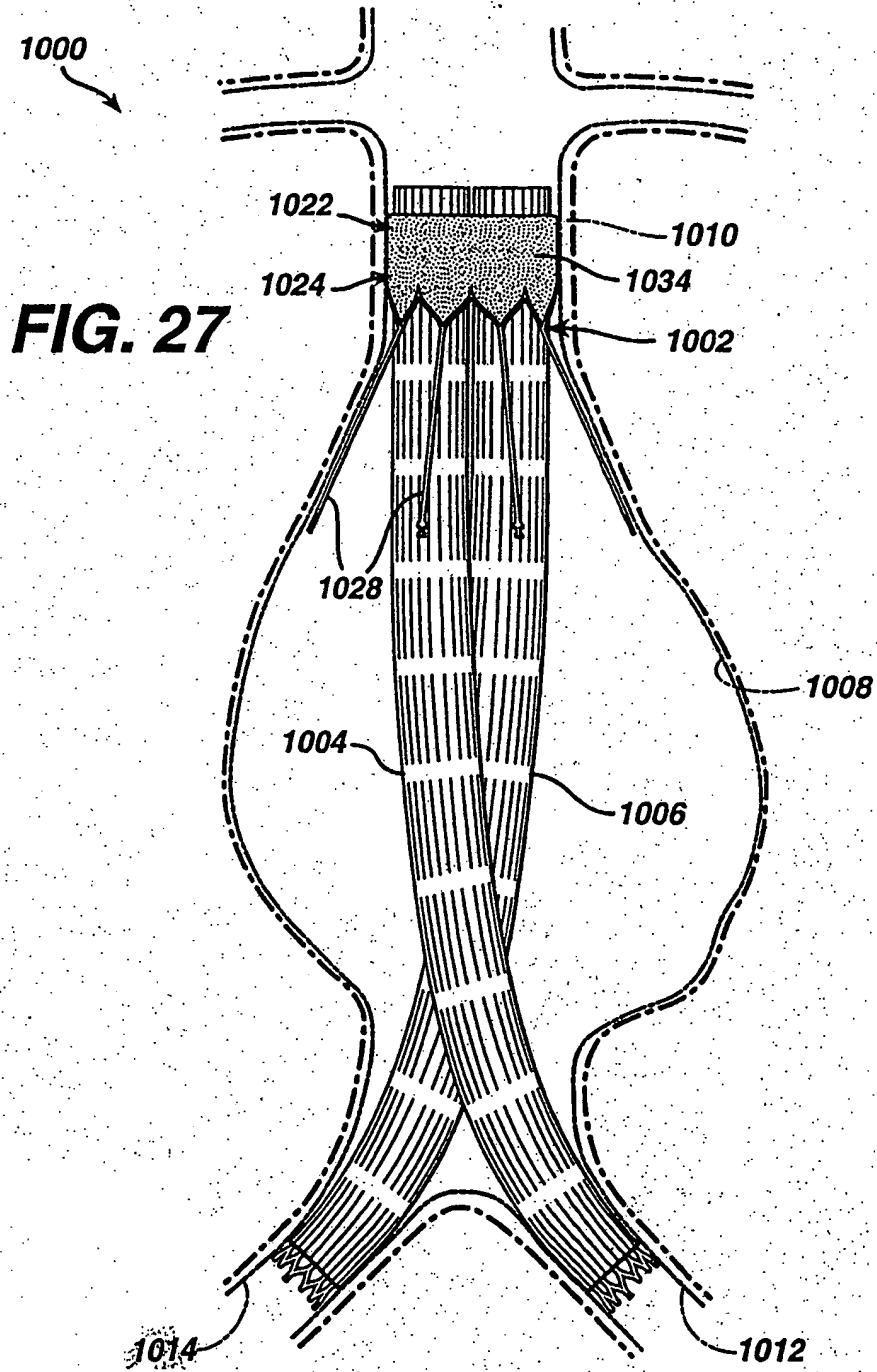


FIG. 28

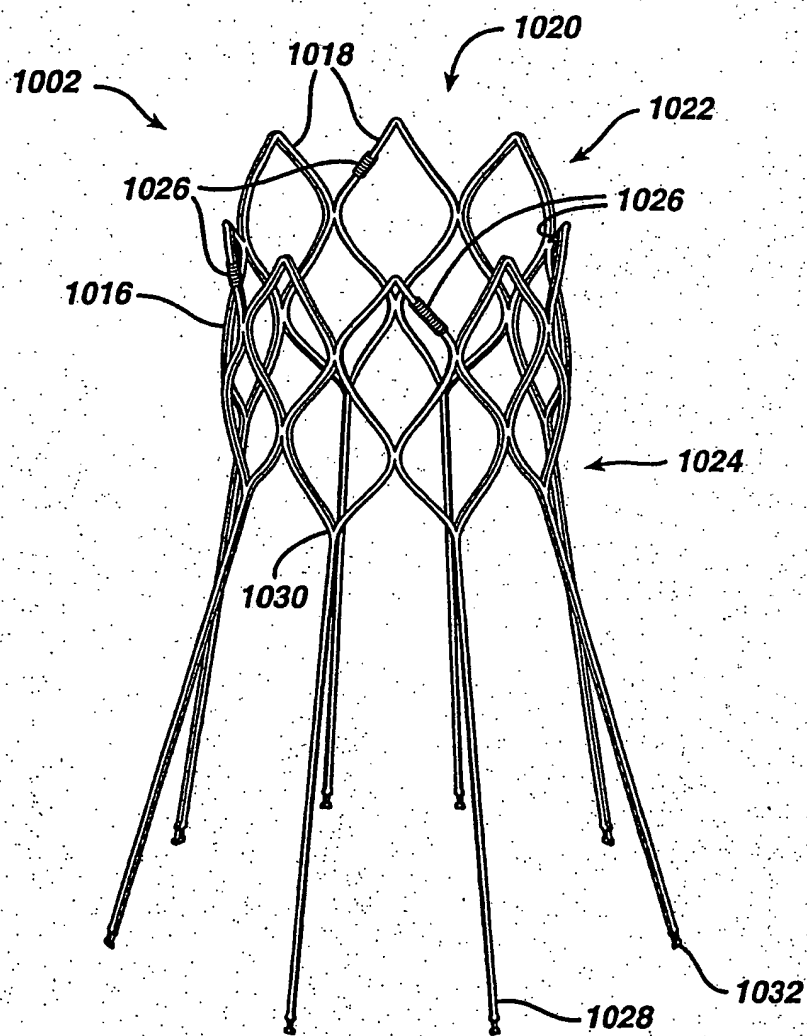
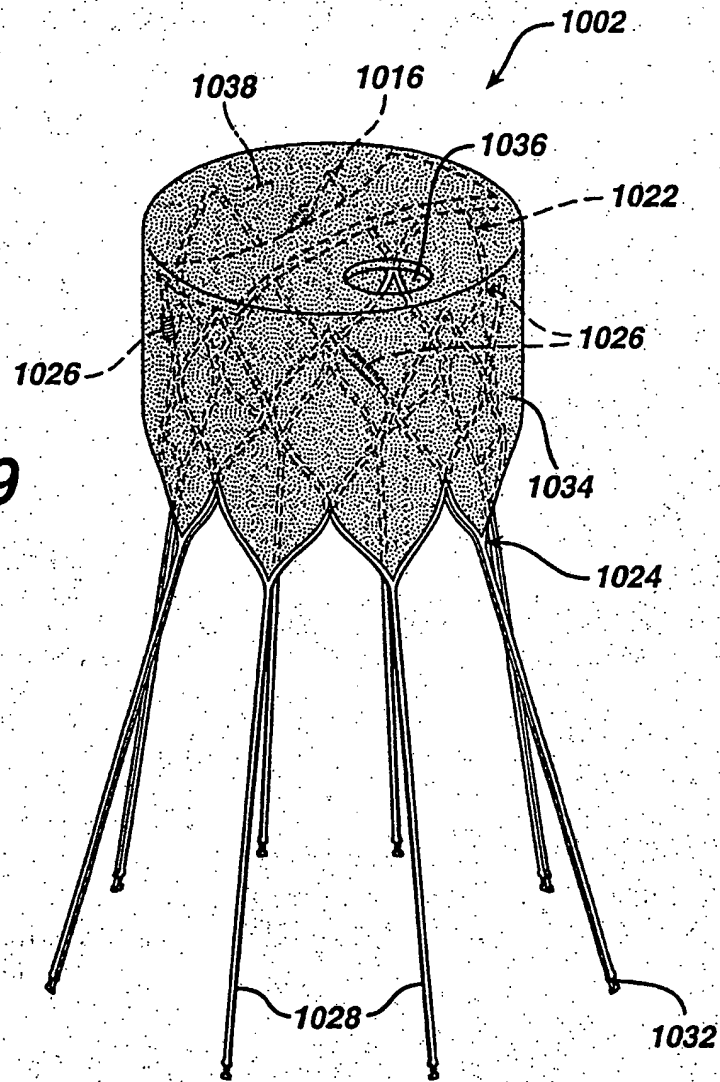


FIG. 29



EP 1 360 967 A1



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 03 25 2701

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (In.CI.7)
X	WO 02 26139 A (CORDIS CORP) 4 April 2002 (2002-04-04) * claims; figures *	1-23	A61L31/10 A61L31/16 A61F2/06
X	WO 01 87375 A (CORDIS CORP) 22 November 2001 (2001-11-22) * claims; figures *	1-23	
P,X	US 2002/058984 A1 (SOLOVAY KENNETH S ET AL) 16 May 2002 (2002-05-16) * claims; figures *	1-23	
A	US 6 245 100 B1 (DAVILA LUIS A ET AL) 12 June 2001 (2001-06-12) * claims; figures *	1-23	
			TECHNICAL FIELDS SEARCHED (In.CI.7)
			A61L A61F A61M
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 16 September 2003	Examiner ESPINOSA, M
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 (03.02.2004C01)

EP 1 360 967 A1

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 03 25 2701

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

16-09-2003

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 0226139	A	04-04-2002	US 2001029351 A1	11-10-2001
			US 2002165608 A1	07-11-2002
			US 2002133183 A1	19-09-2002
			AU 1129902 A	08-04-2002
			AU 1132102 A	08-04-2002
			AU 7730201 A	11-04-2002
			AU 9316101 A	08-04-2002
			AU 9486901 A	08-04-2002
			CA 2357881 A1	29-03-2002
			CA 2424029 A1	04-04-2002
			CA 2424038 A1	04-04-2002
			CA 2424049 A1	04-04-2002
			CA 2425753 A1	04-04-2002
			EP 1192957 A2	03-04-2002
			EP 1335761 A1	20-08-2003
			EP 1322235 A1	02-07-2003
			EP 1322351 A1	02-07-2003
			EP 1322342 A1	02-07-2003
			JP 2002238994 A	27-08-2002
			WO 0226280 A1	04-04-2002
			WO 0226139 A1	04-04-2002
			WO 0226281 A1	04-04-2002
			WO 0226271 A1	04-04-2002
			US 2002094440 A1	18-07-2002
			US 2002111590 A1	15-08-2002
			US 2002051730 A1	02-05-2002
			CA 2408754 A1	22-11-2001
			WO 03000308 A1	03-01-2003
			US 2003065377 A1	03-04-2003
			US 2003065345 A1	03-04-2003
			US 2003065346 A1	03-04-2003
WO 0187375	A	22-11-2001	AU 5977401 A	26-11-2001
			AU 6157901 A	26-11-2001
			AU 6158001 A	26-11-2001
			AU 6158101 A	26-11-2001
			AU 6295701 A	26-11-2001
			AU 6311201 A	26-11-2001
			AU 6311301 A	26-11-2001
			CA 2408606 A1	22-11-2001
			CA 2408608 A1	22-11-2001
			CA 2408719 A1	22-11-2001
			CA 2408729 A1	22-11-2001
			CA 2408752 A1	22-11-2001
			CA 2408754 A1	22-11-2001
			CA 2408838 A1	22-11-2001

EPO FORM P/438

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 03 25 2701

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

16-09-2003

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 0187375 A		EP 1280568 A1	05-02-2003
		EP 1280569 A1	05-02-2003
		EP 1280570 A2	05-02-2003
		EP 1280571 A1	05-02-2003
		EP 1289576 A1	12-03-2003
		EP 1280512 A2	05-02-2003
		EP 1280572 A1	05-02-2003
		WO 0187372 A1	22-11-2001
		WO 0187373 A1	22-11-2001
		WO 0187374 A1	22-11-2001
		WO 0187342 A2	22-11-2001
		WO 0187375 A1	22-11-2001
		WO 0187263 A2	22-11-2001
		WO 0187376 A1	22-11-2001
		US 2001029351 A1	11-10-2001
		US 2002016625 A1	07-02-2002
		US 2002007213 A1	17-01-2002
		US 2002007214 A1	17-01-2002
		US 2002007215 A1	17-01-2002
		US 2002005206 A1	17-01-2002
US 2002058984 A1	16-05-2002	US 6482227 B1	19-11-2002
		CA 2415717 A1	08-07-2003
		EP 1325715 A2	09-07-2003
		AU 8730801 A	23-05-2002
		CA 2363349 A1	16-05-2002
		EP 1208817 A2	29-05-2002
		JP 2002191703 A	10-07-2002
		US 2002058986 A1	16-05-2002
		US 2002058987 A1	16-05-2002
		AU 8731101 A	23-05-2002
		CA 2363311 A1	16-05-2002
		EP 1212987 A2	12-06-2002
		JP 2002191700 A	09-07-2002
		US 2002058985 A1	16-05-2002
		US 2002058993 A1	16-05-2002
		AU 8940501 A	23-05-2002
		CA 2363291 A1	16-05-2002
		EP 1212990 A2	12-06-2002
		JP 2002191701 A	10-07-2002
		AU 8730901 A	23-05-2002
US 6245100	B1	CA 2363314 A1	16-05-2002
		EP 1212988 A2	12-06-2002
		JP 2002191702 A	10-07-2002
		AU 1669601 A	02-08-2001

EPO FORM P/038

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

EP 1 360 967 A1

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 03 25 2701

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

16-09-2003

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6245100	B1	CA 2333339 A1	01-08-2001
		JP 2001245990 A	11-09-2001

EPO FORM P449

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☒ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.